

1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21 22 23 24 25 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 52 53 54 55 56 57 58 59 60 61 62 63 64 65 66 67 68 69 70 71 72 73 74 75 76 77 78 79 80 81 82 83 84 85 86 87 88 89 90 91 92 93 94 95 96 97 98 99 100 101 102 103 104 105 106 107 108 109 110 111 112 113 114 115 116 117 118 119 120 121 122 123 124 125 126 127 128 129 130 131 132 133 134 135 136 137 138 139 140 141 142 143 144 145 146 147 148 149 150 151 152 153 154 155 156 157 158 159 160 161 162 163 164 165 166 167 168 169 170 171 172 173 174 175 176 177 178 179 180 181 182 183 184 185 186 187 188 189 190 191 192 193 194 195 196 197 198 199 200 201 202 203 204 205 206 207 208 209 210 211 212 213 214 215 216 217 218 219 220 221 222 223 224 225 226 227 228 229 230 231 232 233 234 235 236 237 238 239 240 241 242 243 244 245 246 247 248 249 250 251 252 253 254 255 256 257 258 259 260 261 262 263 264 265 266 267 268 269 270 271 272 273 274 275 276 277 278 279 280 281 282 283 284 285 286 287 288 289 290 291 292 293 294 295 296 297 298 299 300 301 302 303 304 305 306 307 308 309 310 311 312 313 314 315 316 317 318 319 320 321 322 323 324 325 326 327 328 329 330 331 332 333 334 335 336 337 338 339 340 341 342 343 344 345 346 347 348 349 350 351 352 353 354 355 356 357 358 359 360 361 362 363 364 365 366 367 368 369 370 371 372 373 374 375 376 377 378 379 380 381 382 383 384 385 386 387 388 389 390 391 392 393 394 395 396 397 398 399 400 401 402 403 404 405 406 407 408 409 410 411 412 413 414 415 416 417 418 419 420 421 422 423 424 425 426 427 428 429 430 431 432 433 434 435 436 437 438 439 440 441 442 443 444 445 446 447 448 449 450 451 452 453 454 455 456 457 458 459 460 461 462 463 464 465 466 467 468 469 470 471 472 473 474 475 476 477 478 479 480 481 482 483 484 485 486 487 488 489 490 491 492 493 494 495 496 497 498 499 500 501 502 503 504 505 506 507 508 509 510 511 512 513 514 515 516 517 518 519 520 521 522 523 524 525 526 527 528 529 530 531 532 533 534 535 536 537 538 539 540 541 542 543 544 545 546 547 548 549 550 551 552 553 554 555 556 557 558 559 560 561 562 563 564 565 566 567 568 569 570 571 572 573 574 575 576 577 578 579 580 581 582 583 584 585 586 587 588 589 590 591 592 593 594 595 596 597 598 599 600 601 602 603 604 605 606 607 608 609 610 611 612 613 614 615 616 617 618 619 620 621 622 623 624 625 626 627 628 629 630 631 632 633 634 635 636 637 638 639 640 641 642 643 644 645 646 647 648 649 650 651 652 653 654 655 656 657 658 659 660 661 662 663 664 665 666 667 668 669 670 671 672 673 674 675 676 677 678 679 680 681 682 683 684 685 686 687 688 689 690 691 692 693 694 695 696 697 698 699 700 701 702 703 704 705 706 707 708 709 710 711 712 713 714 715 716 717 718 719 720 721 722 723 724 725 726 727 728 729 730 731 732 733 734 735 736 737 738 739 740 741 742 743 744 745 746 747 748 749 750 751 752 753 754 755 756 757 758 759 760 761 762 763 764 765 766 767 768 769 770 771 772 773 774 775 776 777 778 779 780 781 782 783 784 785 786 787 788 789 790 791 792 793 794 795 796 797 798 799 800 801 802 803 804 805 806 807 808 809 810 811 812 813 814 815 816 817 818 819 820 821 822 823 824 825 826 827 828 829 830 831 832 833 834 835 836 837 838 839 840 841 842 843 844 845 846 847 848 849 850 851 852 853 854 855 856 857 858 859 860 861 862 863 864 865 866 867 868 869 870 871 872 873 874 875 876 877 878 879 880 881 882 883 884 885 886 887 888 889 890 891 892 893 894 895 896 897 898 899 900 901 902 903 904 905 906 907 908 909 910 911 912 913 914 915 916 917 918 919 920 921 922 923 924 925 926 927 928 929 930 931 932 933 934 935 936 937 938 939 940 941 942 943 944 945 946 947 948 949 950 951 952 953 954 955 956 957 958 959 960 961 962 963 964 965 966 967 968 969 970 971 972 973 974 975 976 977 978 979 980 981 982 983 984 985 986 987 988 989 990 991 992 993 994 995 996 997 998 999 1000 1001 1002 1003 1004 1005 1006 1007 1008 1009 1010 1011 1012 1013 1014 1015 1016 1017 1018 1019 1020 1021 1022 1023 1024 1025 1026 1027 1028 1029 1030 1031 1032 1033 1034 1035 1036 1037 1038 1039 1040 1

**(43) International Publication Date**  
**15 February 2001 (15.02.2001)**

**PCT**

**(10) International Publication Number**  
**WO 01/10313 A1**

(51) International Patent Classification?: A61B 17/22

(21) International Application Number: PCT/US00/20525

(22) International Filing Date: 28 July 2000 (28.07.2000)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
09/368,410 5 August 1999 (05.08.1999) US

(71) Applicant (for all designated States except US): KENSEY NASH CORPORATION [US/US]; Marsh Creek Corporate Center, 55 East Uwchlan Avenue, Suite 204, Exton, PA 19341 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): NASH, John, E. [US/US]; 1201 North Chester Springs Road, Chester Springs, PA 19425 (US). EVANS, Douglas, G. [US/US]; 202 Foxtail Lane, Downingtown, PA 19335 (US). HOGANSON, David, M. [US/US]; 300 East Evans Street, Apartment C302, West Chester, PA 19380 (US).

(74) Agent: STEIN, Barry, A.; Caesar Rivize Bernstein Cohen & Pokotilow Ltd, 12th Floor, Seven Penn Center, 1635 Market Street, Philadelphia, PA 19103-2212 (US).

(81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.


(84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

**Published:**

- With international search report.
- Before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments.

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

**(54) Title: SYSTEM AND METHOD FOR DELIVERING AGENTS INTO TARGETED TISSUE OF A LIVING BEING**

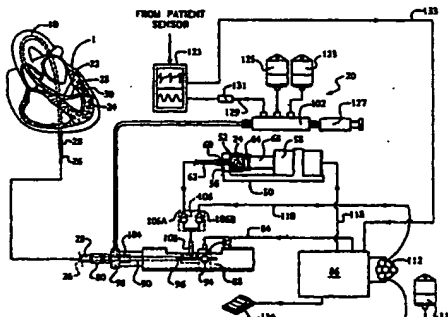

**WO 01/10313 A1**

(57) **Abstract:** The systems basically comprise a delivery system for accessing the targeted tissue within the living being and introduction of at least one agent at select locations into the myocardium and other select tissues. The delivery systems are arranged to access the tissues of the heart. One or more of the systems can be utilized during transluminal, transthoracic and direct surgical access procedures. Where appropriate, for example in the case of intraventricular access, portions of the system are steerable to properly orient the device. The instruments may pierce the heart tissue and create channels extending from the endocardium, the epicardium, or the cardiac vessels. When tissue penetration is utilized, the device may include a feature to control the depth of penetration. To minimize bleeding through the channels the device can dilate small initial punctures that later contract down after device removal. When the formation of channels is required, this can be achieved, by way of example, with a rotary-tipped device, pressurized fluid jet devices, vibratory instruments and piercing needle-like tip devices. The system may utilize some form of mechanical action or application of energy (e.g. electrical, sonic, thermal, optical, pressurized fluid, radio frequency (RF), nuclear) in the process. The mechanical action or energy application may affect the surrounding tissues at a distance from the device. The agent delivered to the tissue may include one or more of pharmaceuticals, biologically active agents, radiopaque materials, etc.

the occluded site. In general, the conduits are either synthetic or natural bypass grafts. Grafting with the internal thoracic (internal mammary) artery directly to the blocked coronary site has been particularly successful with superior long-term patency results. During conventional cardiac surgery, the heart is stopped using cardioplegia solutions and the patient is put on cardiopulmonary bypass. The bypass procedure uses a heart-lung machine to maintain circulation throughout the body during the surgical procedure. A state of hypothermia may be induced in the heart tissue during the bypass procedure to preserve the tissue from necrosis. Once the procedure is complete, the heart is resuscitated and the patient is removed from bypass.

There are great risks associated with these traditional surgical procedures such as significant pain, extended rehabilitation time and high risk of mortality for the patient. The procedure is time-consuming and costly to perform. Traditional cardiac surgery also requires that the patient have both adequate lung and kidney function in order to tolerate the circulatory bypass associated with the procedure and a number of patients which are medically unstable are thus not a candidate for bypass surgery. As a result, over the past few years, minimally invasive techniques for performing bypass surgery have been developed and in some instances the need for cardiopulmonary bypass and extended recovery times are avoided. A number of companies, e.g., Heartport, Inc. of Redwood City, CA and Cardiothoracic Systems, Inc. of Cupertino, CA, have developed devices that allow for cardiac surgical procedures that do not require a grossly invasive median sternotomy or traditional cardiopulmonary bypass equipment. The procedures result in a significant reduction in pain and rehabilitation time.

In addition, as an alternative to surgical methods, traditional interventional cardiology methods (e.g. angioplasty, atherectomy, and stents) non-surgical procedures, such as percutaneous transluminal coronary angioplasty (PTCA), rotational atherectomy, and stenting have been successfully used to treat this disease in a less invasive non-surgical fashion. In balloon angioplasty a long, thin catheter having a tiny inflatable balloon at its distal end is threaded through the cardiovascular system until the balloon is located at the location of the narrowed blood vessel. The balloon is then inflated to separate and expand the obstructing plaque and expand the arterial wall, thereby restoring or improving the flow of blood to the local and distal tissues. Rotational atherectomy utilizes a similarly long and thin catheter, but with a rotational cutting tip at its distal end for cutting through the occluding material. Stenting

utilizes a balloon tipped catheter to expand a small coil-spring-like scaffold at the site of the blockage to hold the blood vessel open.

While many patients are successfully relieved of their symptoms and pain with traditional interventional procedures, in a significant number of patients the blood vessels eventually restenose or reocclude within a relatively short period of time. As such, researchers have explored advanced interventional cardiology methods (e.g., catheter based drug delivery, radiation therapy, etc.) to delay or prohibit the process of restenosis. As summarized by Raoul Bonan, MD ("Local Drug Delivery for the Treatment of Thrombus and Restenosis, IAGS Proceedings, The Journal of Invasive Cardiology, 8:399-408, October 1996), the cardiology community has recently begun to augment standard catheter-based treatment techniques with devices that provide local delivery of medications to the treated site. This localized administration of drugs has shown promise for counteracting clotting, reducing inflammatory responses, and blocking proliferative responses.

Several devices are reported to be under evaluation for site specific drug delivery, such as the so-called "Channel Balloon" catheter of Boston Scientific (Natick, Massachusetts), the "Infiltrator" device of InterVentional Technologies (San Diego, CA), the "InfusaSleeve" device of LocalMed Inc. (Sunnyvale, CA), the "Dispatch" catheter of SciMed/Boston Scientific (Natick, Mass), and an ultrasound enhanced catheter of EKOS (Bothell WA). The "Channel Balloon" catheter is an over-the-wire catheter with separated ports for balloon inflation and drug infusion. The "Infiltrator" device utilizes nipples in a balloon to force a drug into vessel wall.

United States Letters Patent No. 5,279,565 (Klein et al.) discloses a device for infusing a treatment site with a medicinal agent. The device has a flexible body and deflectable support frames that are deployed radially against the intended treatment site. The InfusaSleeve device of LocalMed, Inc. slides over existing balloons to position drug delivery ports against the artery wall. The Dispatch is an over the wire catheter with separate ports for drug infusion and balloon inflation.

United States Letters Patent No. 5,527,292 (Adams et al.) describes an intravascular device having an elongated flexible tube sized for insertion into a coronary vessel beyond a distal end of a guide catheter. In certain applications, the intravascular device is used as a drug (or other fluid) delivery device or as an aspiration device. In other applications, the intravascular device is used as a guiding means for placement of an angioplasty device, such as a guide wire or a balloon catheter. EKOS (Bothell, Washington) has developed a site-specific catheter that

uses ultrasound energy to enhance the performance of a thrombolytic drug. The ultrasound energy transports the drug molecules into the strands of fibrin bundles to dissolve clots more effectively than drugs alone. Several other drug delivery catheters have been described.

Balloon-tipped catheters, appropriate for drug delivery procedures, are also described in United States Letters Patent No. 5,087,244 (Wolinsky et al.). In particular, this patent describes a catheter having a balloon near its distal end is expanded with a medication that then flows through minute holes in the balloon surface at a low flow rate. The catheter pressurizes the medication so that it can be perfused at a controlled low flow rate to penetrate into the wall of the localized tissue.

United States Letters Patent Numbers 5,021,044 (Sharkawy) describes an intravascular treatment apparatus having a plurality of holes on the outer surface of the catheter body through which a drug may be delivered to a site within a vessel.

United States Letters Patent No. 5,112,305 (Barath et al.) describes a catheter for delivery of therapeutic chemical agents to an interior wall of a vessel, the catheter having a balloon near its distal end with tubular extensions projecting from its outer surface. The catheter is pressurized with a drug, which causes the balloon to expand. The drug then flows throughout the tubular extension into the vessel wall.

United States Letters Patent No. 4,406,656 (Hattler et al.) describes a collapsible multi-lumen venous catheter that can be used for drug injection.

United States Letters Patent Numbers 5,498,238 (Shapland et al.) discloses a method of simultaneous angioplasty and drug delivery to a localized portion of coronary or peripheral arteries or any other type of body passage that has a stricture. The drug delivery device is first positioned in a body passageway. The device is expanded in order to dilate the passage while simultaneously causing a selected drug to be transported across a drug transport wall of the device for direct contact with the passageway wall.

United States Letters Patent No. 5,415,637 (Khosravi) describes an intravascular catheter that is capable of delivering a drug, that is in the form of an already mixed solution or in the form of pellets, both intraluminally and endoluminally to an artery.

United States Letters Patent No. (Spears) describes a method for treating a lesion in an artery by bonding a bioprotective material to the arterial wall with thermal energy to provide localized drug delivery. The device can use drugs that are trapped within microspheres that can be thermally bonded to tissues.

United States Letters Patent No. 4,994,033 (Shockey et al.) describes an intravascular treatment apparatus having a pair of expansion members concentrically arranged near its distal end wherein a drug is delivered to the outer expansion member. The expansion member expands against the vessel wall forcing the drug through minute holes in the outer member to bathe the vessel wall.

United States Letters Patent No. 5,456,667 (Ham et al.) describes an intravascular catheter with an expandable region formed of a tubular material at the distal end of the catheter body in a one-piece configuration and is radially expanded and contracted by means of a control wire. The interior of the expandable region is in fluid communication with a lumen in the catheter body to allow the delivery of a fluid to the artery via openings in the surface of the expandable region. The catheter is particularly adapted to hold open an artery after a vascular procedure such as a balloon angioplasty, and if desired to introduce a therapeutic drug or other fluid to the site of the vascular procedure.

The assignee of this present invention is also the assignee of previously described catheter-based devices for the local delivery of drugs into the arterial system. See for example, United States Letters Patent No. 4,589,412 (Kensey) and No. 4,631,052 (Kensey) disclose atherectomy catheters that utilize a cutting tip that is driven by the application of fluid pressure. As described, the catheters can be used to deliver drugs, oxygen, nitrates, calcium channel blockers or contrast media through the catheter tip into the arterial lumen.

United States Letters Patent No. 4,747,406 (Nash) and No. 4,686,982 (Nash), which are assigned to the same assignee as this invention, describe recanalization catheters with a high speed working end that is driven by a flexible drive shaft mounted within a bearing. The specification describes the use of fluid to cool and lubricate the catheter, as well as reduce the incidence of snagging as a result of the positive pressure applied to the artery wall. The fluid can include nitrates, drugs, or contrast media.

United States Letters Patent Nos. 4,664,112 (Kensey), 4,679,558 (Kensey et al.), and 4,700,705 (Kensey), assigned to the same assignee as this invention, describe small diameter catheter devices with a high-speed working head used for dilating lumens and stopping arterial or other lumen spasm. The specifications describe the use of fluids to cool and lubricate the catheter. The fluid can carry contrast media or drugs. The catheters may be useful for opening restrictions in lumens by bombarding the restriction with propelled fluids at high pressure which

may force the liquid into the lumen walls by increasing the local dynamic or hydrostatic pressure induced by the injected liquid or the moving working head.

United States Letters Patent No. 4,790,813 (Kensey), also assigned to the same assignee as this invention, describes an atherectomy catheter that utilizes a cutting tip that is driven by the application of fluid pressure. As described, that catheter has the potential for the delivery of drugs, oxygen, nitrates, calcium channel blockers or contrast media through the catheter tip into the arterial lumen.

United States Letters Patent No. 4,795,438 (Kensey et al.), also assigned to the same assignee as this invention, describes a flexible small diameter catheter for effecting the formation of a restriction in a vessel. The patent teaches of a rotary catheter that is used to deliver fluid, particles, sclerosing liquid, micron-sized particles, and adhesive agents. In one aspect of the invention, the particles are embedded into the tissue contiguous with the working head of the catheter. The embedded particles cause the tissue to change, e.g. form scar tissue, whereupon a restriction is formed. Another aspect of the invention describes the use of abrasive particles to sclerose or abrade tissue.

United States Letters Patent Nos. 4,749,376 (Kensey et al.), 5,042,984 (Kensey et al.), and 4,747,821 (Kensey et al.), all assigned to the same assignee of this invention, describe drive-wire driven rotary catheters for opening an arterial restriction. The devices utilize the rotation of a working head to cause fluid to be thrown radially outward from the working head to impact the artery wall.

In general, these previous devices are suited to deliver drugs and other therapeutic agents locally to the immediate lumen (e.g., artery) wall to address restenosis. However, they do not address the problem of treating other heart tissues (e.g., myocardium) located beyond the arterial wall.

It has been shown that some patients can receive significant benefits from recently developed medical treatments. Some of these treatments are applied to other tissues of the heart (e.g. the myocardium). In addition, although the non-surgical interventional cardiology procedures are much less costly and less traumatic to the patient than traditional coronary bypass surgery, there are a number of patients for which these procedures are not suitable. For certain types of patients the presence of extremely diffuse stenotic lesions and total occlusion in tortuous vessels prohibits them from being candidates for traditional cardiac surgery. For these patients, direct myocardial revascularization has been performed by inducing the creation

vessels), (3) cardiac denervation, (4) the placebo effect, (5) ablation of ischemic myocardium, and (6) formation of collateral circulation.

Currently it is believed that cardiac denervation and angiogenesis are the primary causes for post procedure angina relief and improved perfusion respectively. The injury damages nerves thereby minimizing the pain sensation and stimulates angiogenesis. While the aforementioned techniques and methods for revascularizing the myocardium offer some promise they never the less suffer from one disadvantage or another. As a first example, the lasers are very expensive to purchase. The aforementioned U.S. Patent Application, Serial No. 08/958,788, filed on October 29, 1997 is directed to the same or similar medical benefits achieved by use of non-laser devices, such as those disclosed and claimed therein. As a second example, the design of the interventional cardiology catheter-based drug delivery systems appear unable to delivery drugs to tissues located beyond the arterial walls. Significant benefit could be gained by the delivery of agents (e.g. foreign body particles, drugs, growth factors, genetic material, etc.) into heart tissues beyond the arterial wall. Those devices that have considered direct injection of drugs or genetic material into the myocardium simply deposit the material within a channel that is typically created by a needle. As the myocardium dynamically contracts, deposits of materials in these channels will likely migrate unless stabilized with a mechanical or chemical anchor of some sort. It is the intent of this invention to overcome these and other shortcomings of the prior art.

#### OBJECTS OF THE INVENTION

Accordingly, it is a general object of this invention to provide a system and methods for treating targeted internal tissue, e.g., cardiac tissue or other internal tissue, of a living being which overcomes the shortcomings of the prior art.

It is a further object of this invention to provide a system and method for myocardial revascularization that overcomes the disadvantages of the prior art.

It is a further object of this invention to provide a system and method for vascularizing the cardiac tissue of a living being to cause the formation of lumens in communication with the being's arterial system.

It is a further object of this invention to provide a system and method for treating cardiac tissue of a living being to affect the conduction of electrical signals in the cardiac tissue.

It is a further object of this invention to provide a system and method for treating cardiac tissue of a living being to affect the conduction of nerve signals in the cardiac tissue.

It is a further object of this invention to provide a system and methods for treating targeted internal tissue, e.g., cardiac tissue or other internal tissue, by delivering flowable agent(s) thereto.

It is a further object of this invention to provide a system and methodology for providing relief from myocardial ischemia.

It is a further object of the present invention to provide a system having delivery capabilities delivering agents flowable agents to internal body tissues for beneficial purposes, such as, but not limited to treating heart disease.

It is a further object of this invention to provide apparatus and methods for providing myocardial perfusion that reduce the level of ischemia in a living being.

It is a further object of this invention to provide methods and apparatus for reducing the level of discomfort associated with angina in a living being.

It is a further object of this invention to provide apparatus and methods to enable living beings that suffer from the later stages of ischemic heart disease to experience reduced pain and improved emotional well being.

It is a further object of this invention to provide a transmyocardial revascularization system and methodology that is simple and cost effective.

It is a further object of this invention to provide an apparatus and method for myocardial revascularization to increase blood flow to the myocardium from the endocardium without using the native diseased coronary arteries.

It is a further object of this invention to provide an apparatus and method for myocardial revascularization to be used with living beings having extensive coronary atherosclerosis.

It is a further object of this invention is to provide apparatus and methods for effecting endovascular myocardial revascularization.

It is a further object of the present invention to provide methods and apparatus which can be utilized either in open surgical, minimally invasive surgical, or transluminal techniques to deliver beneficial agents to the myocardium.

It is a further object of this invention to provide a system and method for direct myocardial revascularization without the need for opening the chest cavity.

It is a further object of this invention to provide as system and method for direct endovascular myocardial revascularization without having to utilize a laser, although a laser may be used, if desired, in some applications as part of the procedure.



It is a further object of this invention to provide a system and method to create channels in the myocardium without having to utilize a laser, although a laser may be used, if desired, in some applications as part of the procedure.

It is a further object of this invention to provide a system and method for effecting initial and prolonged stimulus within the myocardium that instigates the heart to heal itself.

It is a further object of this invention to provide instruments with delivery capabilities for dispersing flowable agent(s) into targeted internal tissues of a living being at a location beyond that which is immediately adjacent the instrument.

#### SUMMARY OF THE INVENTION

These and other objects of this invention are achieved by providing tissue, e.g., cardiac, treatment systems and methods of treating tissue, such as the myocardium and other tissues, within the body of a living being.

The treatment system can be used for vascularizing the cardiac tissue of a living being to cause the formation of lumens in communication with the being's arterial system, or can be used to affect the conduction of electrical signals in the cardiac tissue, or can be used to affect the conduction of nerve signals in the cardiac tissue, or in some way beneficially treat other (e.g., non-cardiac) tissue within the body of the being.

To that end the treatment system comprises a delivery instrument and a flowable agent. The flowable agent comprises a plurality of small particles for introduction into the cardiac tissue or other tissue. The delivery instrument is arranged to introduce the flowable agent at or adjacent the cardiac or other targeted tissue by imparting a force to the agent, whereupon the agent directly enters the cardiac or other targeted tissue at an entry situs.

#### DESCRIPTION OF THE DRAWINGS

Other objects and many attendant features of this invention will become readily appreciated as the same becomes better understood by reference to the following detailed description when considered in connection with the accompanying drawing wherein:

Fig. 1A is an illustration of the heart of a living human being, partially in section, showing one embodiment of a delivery instrument forming a portion of the tissue treatment, e.g., myocardial revascularization, system of the subject invention being used to penetrate a portion of the septum to deliver flowable agent(s) to the targeted tissue, e.g., the septum, via the endocardium;

Fig. 1B is an illustration similar to that of Fig. 1A, but showing the embodiment of the delivery instrument being used to penetrate a portion of the myocardium to deliver the flowable agent(s) into the myocardium via the endocardium;

Fig. 2 is an enlarged sectional view of the distal portion of the delivery instrument embodiment illustrated in Figs. 1A and 1B, and showing the flow paths of the agent(s) through and out of the instrument for dispersion into the targeted tissue;

Fig. 3A is an enlarged side sectional view of one embodiment of a rupturable capsule containing a dose of the flowable agent(s) for delivery into the targeted tissue by various delivery instruments of the subject invention;

Fig. 3B is an enlarged side sectional view of one embodiment of a piercable capsule containing a dose of the flowable agent(s) for delivery into the targeted tissue by various delivery instruments of the subject invention;

Fig. 4A is an enlarged side elevational view, partially in section, of the embodiment of the needle access capsule of Fig. 3B, positioned within a capsule injector forming a portion of the delivery instrument of Fig. 1;

Fig. 4B is an enlarged side elevational view, partially in section, of the embodiment of the rupturable capsule of Fig. 3A, positioned within a capsule injector forming a portion of the delivery system of Fig. 1;

Fig. 5A is a schematic diagram and system illustration showing one embodiment of an entire targeted tissue treatment system making use of the delivery instrument of Fig. 1 for delivering the flowable agent(s) into a portion of the myocardium in accordance with the vascularization technique illustrated in Fig. 1B;

Fig. 5B is a schematic diagram and system illustration similar to that of Fig. 5A, but showing an embodiment of the entire targeted tissue system making use of the delivery instrument of Fig. 1 for delivering the flowable agent(s) into a portion of the myocardium via a coronary artery to thereby effect myocardial vascularization;

Fig. 6 is an enlarged illustration of the heart of a living human being, partially in section, showing a portion of the delivery instrument of Fig. 5B being used to deliver the flowable agent(s) into the myocardium via a coronary artery;

Fig. 7 is a side sectional view of one embodiment of an alternative, e.g., a rigid, delivery instrument of the targeted tissue treatment system of this invention shown being used for

effecting myocardial revascularization by piercing the epicardium to create a channel in the myocardium, and deliver the flowable agent(s) therein by pressurizing the agent(s);

Fig. 8 is a side sectional view of one embodiment of another alternative, e.g., a flexible, delivery instrument of the targeted tissue treatment system of this invention shown being used for effecting myocardial revascularization by delivering the flowable agent(s) intravascularly through a vessel, e.g., coronary artery, wall into myocardium;

Fig. 9 is an illustration of the heart of a living human being, partially in section, showing another alternative embodiment, e.g., a vibratory, delivery instrument of the targeted tissue treatment system of this invention shown being used to penetrate a portion of the epicardium and myocardium to deliver the flowable agent(s) into the myocardium;

Fig. 10 is an enlarged side sectional view showing a portion of the vibratory delivery instrument embodiment of Fig. 9 for penetrating tissue and delivering the flowable agent(s) into the myocardium;

Fig. 11 is a schematic diagram and system illustration showing another embodiment of a targeted tissue treatment system of this invention including the embodiment of the vibratory delivery instrument illustrated in Fig. 9 being used to penetrate and deliver the flowable agent(s) to a portion of the myocardium via the epicardium;

Fig. 12 is an illustration of the heart of a living human being, partially in section, showing one embodiment of an alternative delivery instrument forming a portion of the myocardial revascularization system of the subject invention being used to deliver the flowable agent(s) into the myocardium via the epicardium;

Fig. 13 is a side sectional view of the embodiment of the delivery instrument of Fig. 7 with a stabilizing device, e.g., a suction hood, associated with it and shown being used to pierce the epicardium to create a channel in the myocardium and to deliver the flowable agent(s) into the channel in the myocardium;

Fig. 14 is a side sectional view of an embodiment of a delivery instrument, e.g., a flexible pressurized intravascular access delivery instrument, forming a portion of the tissue treatment system of the subject invention being used delivery agents through the urethra wall into the prostate gland of a living being.

Figs. 15A - 15I are embodiments various exemplary types of particulate materials which may make up all or a portion of the flowable agent(s) of the subject invention, in this case the materials being in the form of microspheres and/or microparticles or other small particulates;

Fig. 16 is a side sectional view of one embodiment of a delivery instrument of a targeted tissue treatment, e.g., a myocardial revascularization, system of this invention being used to pierce the epicardium, create a channel in the myocardium, and deliver the flowable agent(s) into myocardium whose vasculature has been reduced over time by atherosclerosis;

Figure 17 is an illustration, like that of Fig. 16, but showing the myocardium immediately after the introduction of the small particles of the flowable agent(s) into the channel in the myocardium followed by the placement of an insert into the channel to increase the vasculature of by the myocardium by the creation of new vessels, e.g., capillaries, in the myocardium;

Figure 18 is an illustration like that of 17, but showing the myocardium some time after treatment by the system of Figs. 16 and 17 where the deployed particles and insert have stimulated angiogenesis to improve the blood flow in the contiguous portion of myocardium;

Figure 19 is an illustration of a portion of the heart of a living being, shown partially in section, and showing a flowable treatment agent delivery system like that of Figure 7 delivering the agent(s) at plural locations to result in the production of an intramyocardial channel for providing an enhanced blood supply to ischemic myocardial tissue;

Figure 20 is an illustration of the portion of the heart shown in Figure 19 after the treatment procedure as depicted therein;

Figure 21 is an enlarged sectional view of the distal or working end of yet another alternative delivery instrument of the targeted tissue treatment system of this invention; and

Figure 22 is an enlarged sectional view of the distal or working end of still another alternative delivery instrument of the targeted tissue treatment system of this invention.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

Referring now to the drawing wherein like reference characters refer to like parts, there is shown in Fig. 1A the distal portion of a delivery subsystem 22 which will be described later and which forms a portion of a tissue treatment, e.g., revascularization system, 20 constructed in accordance with this invention.

These and other objects of this invention are achieved by providing tissue, e.g., cardiac tissue, treatment systems and methods of treating tissue, such as the myocardium and other tissues within the body. The systems basically comprise a delivery system for accessing a targeted tissue within the living being and a flowable agent (to be described in considerable detail later) arranged to be introduced into the targeted tissue by the delivery system.

In several preferred embodiments shown and described herein the tissue treatment system introduces the flowable agent into select portions of the myocardium, or other cardiac tissue.

As will be described later one or more of the delivery systems of this invention can be utilized during transluminal, transthoracic and direct surgical access procedures. Where appropriate, for example in the case of intraventricular access, portions of the delivery system are steerable to properly orient the delivery instrument. In some embodiments the delivery instruments are arranged to pierce the heart tissue and create channels extending from the endocardium, the epicardium, or the cardiac vessels. When tissue penetration is utilized, the delivery instrument can include a feature to control the depth of penetration. To minimize bleeding through the channels the delivery instrument can dilate small initial punctures that later contract down after device removal. When the formation of channels is required, this can be achieved, by way of example, with a rotary-tipped device, pressurized fluid jet devices, vibratory instruments and piercing needle-like tip devices.

The tissue treatment systems of this invention may utilize some form of mechanical action or application of energy, e.g., electrical, sonic, thermal, optical (e.g., laser), pressurized fluid, radio frequency (RF), nuclear, in the process. The mechanical action or energy application may affect the surrounding tissues at a distance from the delivery system. For example, thermal energy may be conducted away via nerve conduits thereby disabling the nerves and creating a condition of denervation. As another example, shockwaves created by sonic energy may travel through the tissue and serve to initiate a change that is beneficial to the patient either immediately or over time.

The delivery instruments may make use of a device to stabilize a portion of the system or anatomy during the procedure (e.g., a vacuum stabilizer or surgical stabilizer ring). A controller may also be provided as part of the system to coordinate the operation of the delivery instrument with the cardiac cycle. For example, power to the delivery instrument can be synchronized with EKG leads, such that delivery instrument operation occurs at a recurring portion of the cardiac cycle.

Radiopaque contrast media, fluoroscopy, ultrasound, magnetic resonance, GPS-like triangulation, RF triangulation, flashback or other imaging/position systems can be used to orient/position the delivery instrument during the procedure. Robotics could also be used to position the delivery instrument of the system in a body cavity or lumen. For example, a robotic

arm can be used to navigate within the chest cavity through a small thoracic incision to position the delivery instrument in relation to the epicardium.

In some applications, the delivery instrument is arranged to directly deliver the flowable agent(s) into the cardiac tissue. In other applications a pressurized system imparts kinetic energy to the flowable agent(s) for the purpose of dispersing the agents into the tissue located beyond the tissue immediately adjacent the delivery instrument of the system. Control parameters on the delivery instrument (e.g. a pressure limiter) can provide control over agent penetration depth.

In some applications the dispersal pattern for the flowable agent(s) can be selected and adjusted to provide for an optimum dispersion of the agent into the targeted tissue.

In applications, the pressurized system of the delivery instrument delivers the agents from the coronary vessels, the endocardium or the epicardium into the myocardium without the need to pierce the tissues of the artery, endocardium or epicardium. The delivery instrument can use a gas, fluid, gel, or other suitable carrier to transport the flowable agent through the instrument and into contact with the tissue.

Although the preferred embodiment of the system will allow delivery of the agents into distant tissues, it may be beneficial to deposit some of the agents within an instrument created channel or to deliver a portion of the agent systemically via the circulatory system. Agents can pre-dosed in per-use packages or the system can draw doses of pre-selected volumes from a reservoir. The system can vary the concentration of the agent in a fluid, or other suitable carrier.

In accordance with some preferred embodiments of this invention the flowable agents are formed of at least one material that can elicit a beneficial response within the tissues. For example, at least a portion of the agents can be comprised of such items as a pharmaceutical, a growth factor, a suitable biomaterial, or a genetic or cellular based material. The presence of the agent can initiate a bio-chemical/biological process that stimulates the tissue to heal itself. The agents can also trigger the onset of a foreign body or healing response to cause the formation of lumens in communication with the arterial system.

The flowable agents can be designed to assist the tissue in functioning more effectively. For example, the agents could contain an electrically conductive element that modifies or improves the contractile motion of the myocardium. It is contemplated that the mere presence of even an inert agent in the tissue may also be beneficial to a living being. Thus, for example,

one embodiment of the invention described herein can be used to deliver a select agent from within the urethra through the urethra wall and into the sphincter muscle to bulk up the sphincter as a remedy for urinary incontinence. As another example the system could be used to overcome the difficulty of transporting pharmaceuticals across the blood-brain by providing positioning a portion of the system in the vicinity of the targeted tissue (e.g., brain tumor) and delivering beneficial agents. As yet another example, the system of the subject invention could be used to disperse beneficial agents (e.g. gene-based elements) into the musculature of a patients with degenerative muscle diseases (e.g., muscular dystrophy).

The flowable agents may be totally resorbable, partially resorbable or non-resorbable. As an example they can be made of polymers, metals, elastomers, glass, ceramics, collagen, proteins or other suitable materials or a combination materials. A collection of agents with varying characteristics (e.g. density) can be delivered to the tissue to allow for a graduated deposition of varying types of agents to different depths of the tissue. Other agent characteristics (e.g. texture and abrasiveness) can be controlled to allow for varying degrees of trauma to encountered tissues. Where the agents incorporate a solid component, the shape of the component can be varied from spheres to fibers to any other desired shape. A form of a microsphere may be utilized to treat the desired tissue region either by occupying space or by stimulating a biological response to the presence of them material or the release from the material of some chemical or biological element.

In the treatment of cardiac tissue, the presence of the flowable agents of this invention when deployed in the myocardium will not appreciably restrict the cardiac contraction of the heart.

The flowable agents may be constructed to effect a time-phased delivery of active ingredients. In summary, both the creation of channels and the dispersion of the agents is designed lead to improvements in patients with cardiovascular disease as a result of: (1) angiogenesis (stimulation of the creation of new blood vessels), (2) cardiac denervation (3) ablation of ischemic myocardium, and (4) formation of collateral circulation.

Turning now to Fig. 1A, there is shown a portion of a cardiac vascularization system 20 in the process of revascularizing the myocardium of a living, e.g., human, being. The entire system 20 is shown in detail in Fig. 5A and will be described in detail later. Suffice it for now to state that the treatment system 20 includes various components and subsystems which cooperate to effect the delivery of flowable agents into relevant tissue of the being, e.g., the

heart, the vascular system, etc. Fig. 1A is an illustration, not to scale, of a section of a healthy, human heart 1. As can be seen, the heart includes the epicardium 2, the myocardium 3, the endocardium 4, the left ventricle 5, the right ventricle 6, the ventricle septum 7, the aortic valve 8, the mitral valve 9, and the aorta 10. As can be seen clearly in Fig. 1A, the distal portion of the delivery subsystem 22 of system 20 is shown penetrating the ventricle septum and delivering the flowable agent(s) 24, which are denoted by the arrows in that illustration, into the adjacent tissues of the septum. The subsystem 22 includes a delivery instrument 26 and a conventional, e.g., Judkins, guiding catheter or instrument 28. The delivery instrument 26 of this embodiment basically comprises an elongated catheter having a high-speed, rotary working head 30 located at the distal end thereof. The guiding instrument 28, which will be described later, is positioned to guide the delivery instrument 26 to the desired location at the ventricle septum. The high speed working head 30 of the delivery instrument is arranged to propel and disperse the flowable agent into the adjacent tissue. The flowable agent may be any type of flowable material, e.g., a fluid that alone or in combination with other additives such as drugs, growth factors, biocompatible microparticles, etc., is to be introduced into the relevant tissue for a desired purpose. The details of various of the flowable agents will be described later. When the delivery instrument 26 is operated, its working head, e.g., the rotary working head of the embodiment described heretofore, or other types of working heads, ejects or bombards the surrounding tissue with the propelled flowable agent(s) 24 at high pressure to force the agent(s) into the tissue by increasing the local dynamic or hydrostatic pressure induced by the agent or the rotating working head. The construction of the delivery instrument 26 allows the agent(s) 24 to be delivered and dispersed into a significant volume of cardiac tissue.

It is important to note at this juncture that most prior art systems for delivering medications to the heart do so either systemically by vein or regionally, e.g., intracoronary infusion. Systemic delivery is not efficient for the treatment of locally isolated disease for various reasons, namely:

a wide range and large number of sites are exposed to the material, large quantities of the agent are required, due to the entire volume of distribution, to obtain the desired effect, and the agent degrades and can be eliminated by various organ systems that keep the agent from reaching the target site, thereby reducing the agent residence time in the body.

As utilized in this invention, local intra-tissue delivery of the flowable agent(s) 24 eliminates these problems. In particular, the flowable agent(s) is (are) distributed into the target



tissue and not just deposited into the channel or puncture created in the tissue. The nature of the pressurized flowable agent carries it to intra-cellular sites beyond the site of the initial puncture.

As will be appreciated by those skilled in the art, penetration into the target tissue is a function of the mass, density and speed of the agent(s). The agent(s) is (are) less likely to migrate away from the site of implantation. When the treatment of the site is complete, the delivery instrument 24 can be repositioned and the procedure repeated to impregnate a new treatment site with the selected agent(s).

It is believed that the systems of the subject invention may be used as sole therapy for end-stage heart disease patients that are not amenable to alternative therapies, such as coronary artery bypass surgery, or the systems could be used as an adjunctive therapy in addition to other cardiac therapies such as PTCA, stenting, or coronary artery bypass surgery.

Fig. 1B illustrates a portion of a transmyocardial revascularization system 20 like that shown in Fig. 1A and constructed in accordance with this invention and shown in the process of revascularizing the myocardium 3. In this illustration, the guiding instrument 28 is positioned to guide the delivery instrument 26 toward the desired location on the myocardium adjacent the left ventricle. The distal portion of the delivery instrument 26 is shown penetrating the myocardium and delivering the agent(s) 24, which are also denoted by the arrows, into the adjacent tissue of the myocardium.

Fig. 2 is an enlarged sectional view of the distal end portion of the delivery instrument 26 which is illustrated in Figs. 1A and 1B, and showing the tissue penetrating system, utilizing the flow path of the agent(s) 24 through and out of the instrument. In accordance with one preferred embodiment of this invention, the instrument is constructed in a fashion similar to those described in United States Letters Patent Nos. 4,747,821 which is assigned to the same assignee as this invention and whose disclosure is incorporated by reference herein. To that end, the working head 30 is a rotary member which is arranged to revolve at a high speed in a bush 32 driven by a double helical drive wire 34 from a remote, proximally-located motor or turbine (not shown). The bush 32 is mounted on the distal end of a flexible or rigid catheter jacket 36. The agent(s) 24, under distribution, is delivered to the proximal end of the delivery instrument 26 (not shown) and is transported down a central passageway therethrough alongside and between the helical drive wires 36 to the bush 34, where the agent(s) 24 passes out of plural grooves 38 provided in the center and end of the front portion of the bush, whereupon the

agent(s) is further energized as it is centrifuged by the rotation of the working head. The working head is arranged to revolve over a conventional guide wire 40, if one is needed for the procedure. The bush 34 is held in place at the distal end of the jacket by a retention band 42. A liner sleeve 44 extends down the center of the double helical drive wires 36. The distal end of the drive wires are fixedly secured, e.g., welded to a central shaft 46 of the working head 30. The distal end of the working head is a generally dome-shaped cam member having flatted or relieved surfaces 48.

Figs. 4A and 4B show two examples of delivery injectors forming a portion of the system 20 for propelling the flowable agent(s) 24 into any of the delivery instruments of this system, such as the delivery instrument 26 described heretofore. In particular, Fig. 4A shows a device 50 for propelling the agent(s) 24 from a rupturable, capsule 52. The injector 50 basically comprises a base plate 54 on which are mounted a capsule receiver 56 and a jack assembly 58. A needle 60 and associated tubing 62 forming a subassembly are mounted in the receiver 56. The tubing 62 is connected to a "highest wins valve" (to be described later) forming a portion of the system 20 for providing the flowable agent(s) to the delivery instrument 26 at the proximal end thereof. Another tube or conduit (also to be described later) is in fluid communication with the highest wins valve and the interior of the delivery instrument 26 so that the flowable agent(s) which will be provided through the tubing 62 enters into the instrument 26 flows therealong, as described above, and exits out of the instrument at the working head.

An enlarged view of the capsule 52 is shown in Fig. 3A. Thus, as can be seen therein, the capsule 52 comprises a container 62, made of a plastic such as polypropylene, and has a piston 64 at its proximal end. The piston 64 is made from a rubber compound similar to that used in medical syringes, and fits firmly, but slidably, in the container 62. On the distal end of the container 62 is a rubber coating 66 which seals the agent(s) 24 within the capsule 52. The coating may also be located along the walls of the container 62, such as shown in Fig. 3A.

Referring again to Fig. 4A, it can be seen that in use the capsule 52 is placed into a recess within the receiver 56 of the delivery injector and the piston 64 is driven toward the distal end of the capsule by a ram 68 of the jack assembly 58. This causes a sharp piercing end portion of the needle 60 in the delivery device 26 to pierce the rubber 66 whereupon the flowable agent(s) 24 flows into the delivery device 26 via the tubing 62 at a pressure determined by the rate of travel of the ram 68 and the impedance of the distal located passageways, e.g., the

tubing 62, the passageway through the instrument 26, and the outlet delivery ports (e.g., the grooves 38 at the working head 30 - see Fig. 2).

Fig. 4B shows a similar injector device 70 for propelling the agent(s) 24 from the capsule 72. The injector 70 is virtually the same as the injector 50, except that it doesn't include a needle 60. Thus, as can be seen, the injector 70 basically comprises a base plate 54 on which are mounted the capsule receiver 56 and the jack assembly 58. A tubing assembly 56 including tubing 62 is mounted on the receiver 56.

An enlarged view of the capsule 72 is shown in Fig. 3B. Thus, as can be seen, that capsule comprises a container 62, made of plastic such as polypropylene, having a piston 64 at its proximal end. The piston is made from a rubber compound similar to that used in medical syringes and fits firmly, but slidably, in the container 62. On the distal end of the container is bonded a thin, frangible disk 74. The disk 74 is formed of aluminum foil or a similar material and is coated with a plastic, such as polyethylene, on its agent-contacting side (the inside). The disk serves to seal the agent(s) 24 within the capsule 62. The coating on the disk also acts as a hot-seal medium when bonding the disk to the container.

Referring again to Fig. 4B, in use the capsule 72 is placed into a recess within the receiver 56 and the piston 64 is driven toward the distal end of the capsule 72 by the ram 64 of the jack assembly 58. As the pressure of the agent(s) 24 rises, the disk 74 ruptures and the agent flows through the associated port into the tubing 62 and the associated instrument 26 at a pressure determined by the rate of travel of the ram and the impedance of the distal tubing and delivery ports, like that described earlier.

Fig. 5A is a schematic diagram and system illustration showing one embodiment of the entire system 20. That system includes not only the guide instrument 28 and the delivery instrument 26 but also means to control the operation of the delivery instrument in accordance with the subject invention. The illustration of Fig. 1B shows only a portion of the system 20 used to penetrate and deliver agent(s) 24 to a portion of the myocardium via the endocardium, whereas the illustration of Fig. 5A shows the entire system for achieving that end.

As mentioned, the delivery instrument 26 is a rotary device, whose distal end is shown in detail in Fig. 2. The device 26 is arranged to pass through the conventional guide catheter 28, which in this application is preferably a steerable, guide catheter. That catheter has a "J" shaped distal end and a knob 80 at the proximal end which used to steer the "J" shaped distal end as shown in Fig. 5A. The details of the steering mechanism are not shown in the drawing

nor will be described hereinafter, but may comprise any suitable means for achieving such steering action, such as that disclosed in United States Letters Patent No. 5,674,197 (van Muniden et.al.), whose disclosure is incorporated by reference herein. The "J" shape of the distal end of the guide catheter 28 permits the user to advance the delivery instrument 26 to the desired position against the endocardium and by rotation of the guide catheter about its longitudinal axis via the knob 80, the "J" shaped distal end can be directed to any area of the ventricle 5.

The rotary working head 30 of the instrument 26 is driven by the drive cable from a turbine 82, via compressed nitrogen provided through a line 84. The line 84 is coupled to a controller 86, whose construction and operation will be described later, which receives compressed nitrogen from a tank or other source (not shown). The turbine 82 is mounted in a cradle 88. The turbine 82 includes an output shaft which is connected via any suitable means (not shown) to the proximal end of the drive helices 34. The turbine 82 is connected to the proximal end portion 90 of the jacket 36 of the instrument 26 so that longitudinal movement of the turbine causes concomitant movement of the instrument 26. To that end, the turbine 82 is slidably mounted in the cradle 88 in a manner which permits the user to feed the delivery instrument 26 down the guide catheter 28 to the precise location by moving a knob 94 connected to the turbine to and fro in a longitudinally extending slot 96 in the cradle 88.

The steerable guide catheter 28 is coupled at its proximal end to a distal manifold 98, which in turn is connected via line 100 to a conventional angiographic manifold 102. The distal end portion of the instrument 26 extends through a conventional hemostasis valve 104 to prevent the egress of blood from the interior of the guide catheter.

The angiographic manifold 102 is a conventional device such as that commonly used in laboratories and thus will not be described in detail. It will suffice to say that the physician uses the manifold 102 to pass a contrast medium via the guide catheter 28 to the site of the delivery instrument's distal or working head 30 in the ventricle for assessment of the location of the guide catheter and the delivery instrument by fluoroscopy.

The flowable agent(s) 24 to be delivered by the delivery instrument 26 is provided in the capsule 62. The capsule is in turn mounted in the injector 50. The agent delivery tube 62 is connected to one input 106A of a conventional "highest wins" valve 106. The outlet from the valve 106 is connected via a line 108 into a port in communication with the interior passageway

extending longitudinally through the jacket of the delivery instrument 26. The other input 106B to the valve 106 is provided via a line 110 from a peristaltic pump 112.

The controller 86 is an electrically powered device which is arranged to accept inputs from a two-position foot control switch 114 to drive the peristaltic pump. The peristaltic pump is connected via a line to a bag or supply of saline 116. The electrically powered controller 86 is arranged to provide power via line 118 to the ram 58 of the injector 50. In addition, as noted earlier, the controller 86 provides the compressed nitrogen via line 84 to the turbine 82 of the delivery instrument.

In use, the guide catheter 28 is extended from the patient entry situs, e.g., the femoral artery, through the vascular system under fluoroscope vision until its distal end is in the appropriate location within the ventricle. The delivery instrument 26 is then advanced through the guide catheter until its working head 30 at its distal end is adjacent the ventricular wall. The foot control switch 114 is then depressed by the operator to a first switch position to cause the turbine 82 of the delivery instrument to operate, whereupon saline from the bag 116 is delivered to the instrument. In particular, the saline is pumped by pump 112 into communicating line 110, through the input line 106B of the highest wins valve 106 and its communicating outlet line 108 into the interior passageway of the delivery instrument. From there it flows longitudinally down the central passageway whereupon it exits from the distal end or at the working head. The operation of the turbine effects the concomitant high speed rotation of the working head. The operator then grasps the slide knob 94 on the cradle 88 and pushes it forward while the working head is rotated at the high speed to advance the working head into the myocardium. The cam surfaces on the working head engage the myocardium tissue to form a bore or channel therein. Preferably, the channel is made approximately one centimeter deep by the advancement of the instrument with respect to the catheter. This action is accomplished rather quickly, e.g., in about five seconds. Once the channel or bore is completed, or during the time of its formation, the foot control switch 114 is depressed by the operator further to the second switch position. This action results in electric power being provided via the controller 86 to the injector 50. In particular, electrical power is provided via line 118 to the jack of the controller, whereupon the jack commences inward movement, thereby causing immediate delivery of the agent(s) 24 into the tubing (the pushing of the ram causes the capsule to be pierced by the piercing needle 60 whereupon the agent flows through the needle into the communicating tubing 62, through the inlet port 106A of the highest wins valve (since this is port will now be at a higher pressure level

than port 106B), whereupon the flowable agent will flow through communicating outlet line 108 into the interior of the delivery instrument 26 at the proximal end thereof. The agent is delivered down the delivery instrument to the working head either by continued motion of the ejector (assuming the capsule charge is large enough) or is carried forward by the continuing flow of saline from the pump 112. It is expected that the delivery of the agent(s) 24 from the capsule to the bore within the myocardium be delivered quite quickly, e.g., in five seconds or less.

In accordance with one preferred use of the system of the subject invention, e.g., the vascularization of the myocardium, plural bores, lumens or channels are formed in the myocardium by repeating the procedure as set forth above. As should be appreciated by those skilled in the art, the number of bores or channels, their size (e.g., inner diameter and depth), their spacing, and the tissue area encompassed thereby will be a matter of choice based on the desires of the operator of the system and the particular tissue treatment desired. For myocardial vascularization applications of this invention it is contemplated that the bores or channels created be within the range of 1/4 to 3 mm in diameter, extending in depth from 1 - 20 mm, and being spaced from one another by 0.25 cm to 5 cm. The area coverage of cardiac tissue encompassed by the bores or channels may be from 1 to 100 square centimeters. Moreover, the size of the particles forming the flowable agent(s) or included in the flowable agent(s) will, of course, be a factor in the determination of the dimensions, spacing and geographic extent of the channels in the targeted tissue.

If it is desired to time the introduction of the delivery system and the flowable agent(s) 24 into the myocardium to any particular portion of the patient's cardiac cycle (e.g., during diastole) then the system 20 preferably includes a cardiac cycle monitor 121 for providing EKG and BP output signals in response to signals provided from associated cardiac sensor(s), e.g., skin-mounted electrodes (not shown) on the patient. As can be seen in Fig. 5A the cardiac cycle monitor 121 is arranged to provide signals, via a line 133, to the controller 86, in response to the monitored cardiac cycle of the patient. The controller 86, in turn, controls the operation of the injector 50 to the delivery instrument 26 in coordination with the sensed cardiac cycle. Thus, the controller 86 can be used to initiate operation of the system to deliver the flowable treatment agent(s) into the myocardium at a predetermined point in the cardiac cycle.

If angiographic placement of the delivery instrument 26 is required, the system 20 preferably includes the heretofore identified manifold 102 as well as associated components,

such as a bag of a contrast medium 123, a bag of saline 125, and a syringe 127 for delivery of a bolus of the contrast medium through the guide catheter 28 via the conduit or line 100. A blood pressure transducer 131 is also provided connected via a line 129 to the manifold. The transducer 131 provides blood pressure signals to the monitor 121.

In Fig. 5B there is shown an illustration of a system for deploying the flowable agent(s) 24 into the wall of a coronary blood vessel, such as the left anterior descending (LAD) artery 11. Thus, the illustration in Fig. 5B is identical to that as shown in Fig. 5A except for the positioning of the guide catheter 28 and the delivery instrument 26 in the left anterior descending coronary artery of the heart.

In this application, the delivery instrument 26 is passed through the guide catheter 28 to the LAD where it distributes the flowable agent(s) 24 into the wall of the LAD by ejecting the agent(s) at a high velocity. This is accomplished by the combination of pressure and the rotary centrifugal action of the working head. To that end, the instrument 26 is inserted into the guide catheter 28 and moved to a location just inside the guide catheters distal tip under fluoroscope vision. The operator of the system then depresses the foot control switch 114 to the first position, whereupon nitrogen flows to the turbine 82 which in turn rotates the working head 30 at the distal tip of the instrument. The operator then advances the instrument longitudinally by sliding the knob 94 in the slot in the cradle until the working head is advanced to the appropriate location in the vessel. The foot switch 114 may then be depressed in the second position, whereupon the capsule ejector ram 68 is driven smartly into the capsule, thereby causing the needle to pierce into the capsule so that the agent(s) 24 flows through the tubing 62 into the input 106A of the highest wins valve 106 and from there through the outlet tube into the interior of the instrument 26. The instrument is then delivered down the instrument to the instrument's working head either by continued motion of the injector (assuming the capsule charge is large enough) or is carried forward by the continuing flow of saline from the peristaltic pump 112. In any case, the flowable material is forced out in a somewhat radial direction, such as shown by the arrows in Fig. 5B whereupon it passes through the artery wall and into the contiguous tissue of the myocardium.

Fig. 6 is an enlarged portion of the illustration shown in Fig. 5B. Thus, it can be seen that when the delivery instrument is located so that it is within the desired coronary artery, e.g., the left anterior descending (LAD) artery 11, its distal end portion extends beyond the distal end of the guide catheter and lies approximately centered within the artery and parallel to the

longitudinal axis thereof. Operation of the instrument 26 causes the tip to bombard the surrounding tissue with the propelled fluids (e.g., the agent(s) 24 with or without saline or other flowable materials at a high pressure). This action forces the flowable liquids into and through the artery wall and into the immediately adjacent myocardium tissue. This is achieved by increasing the local dynamic or hydrostatic pressure induced by the injected flowable materials and/or the movement, e.g., rotation, of the working head. The construction of the instrument allows the flowable agent(s) to be delivered and dispersed into a significant volume of cardiac tissue. As will be described in considerable detail later, the flowable materials or agents may be in the form of fine particulates, e.g., microspheres, which, when dispersed into the cardiac tissue cover a relatively wide area, yet are resistant to further migration, thereby retaining their beneficial effect within the desired portion of the heart.

Fig. 7 is an illustration of a portion of the heart of a living human being, shown partially in section and showing an alternative embodiment of the delivery instrument of the subject invention for introducing the flowable agent(s) 24 therein. In the embodiment shown in Fig. 7, the delivery instrument is designated by the reference number 200 and is in the form of a jet injector. The instrument is used to deliver into the myocardium the flowable materials via the epicardium. To that end, the instrument utilizes a pressurized stream of fluid to distribute the flowable agent(s) into the targeted tissue.

The use of pressurized fluids for medical applications has been known for some time for various applications. For example, pressurized fluids have been used in the past to ablate and remove substances from the body. See for example United States Letters Patent No. 1,902,481 (Pilgrim). This patent discloses the use of a pressurized fluid or medicant to flush undesirable substances from body cavities of animals. United States Letters Patent No. 3,930,505 (Wallach) discloses a surgical apparatus for the removal of tissue from the eye of a patient by making use of a low pressure, e.g., 15 to 3500 psi jet, to disintegrate that tissue. Particles, such as salt crystals, may be introduced into the jet. A suction pump is used for material removal. United States Letters Patent 4,690,672 (Veltrup) discloses a low pressure, e.g., less than 450 psi water jet for ablating deposits. A vacuum pump is also used for evacuation of the fragmented material which is ablated. United States Letters Patent No. 5,496,267 (Drasler) discloses a device for the ablation and removal of thrombus deposits from tissue walls of patients by means of a high pressure jet, e.g., 5,000 to 50,000 Psi. The device of that patent may be used to infuse drugs, inject contrast media for visualization and flush the vessel. United States Letters Patent No.



5,037,432 (Molinari) discloses an apparatus utilizing pressurized fluid in conjunction with an abrasive reducing substance for removing surface portions of human tissue. The device allows a controlled application of a reducing substance for the purpose of obtaining a superficial abrasion of surface portions of the human tissue. This patent does not contemplate utilizing the system for a surgical or percutaneous tool, nor the delivery of a substance into the tissue.

The delivery instrument 200 shown in Fig. 7 is arranged to drive the flowable agent(s) 24 at high pressures into the myocardium and thus implant the agent(s) at some significant distance from the instrument's distal end 202, as indicated by the arrows in this figure. The instrument 200 is a generally rigid or partially rigid device for use in open heart surgery or for use in mini-open heart surgery through a thoracotomy. Like the instrument 26 described heretofore, the delivery instrument 200 is arranged to drive the flowable agent(s) 24 at high pressures into the myocardium 3 to thereby implant that agent at some significant distance from the instrument's distal or working end. However, unlike the delivery instrument 26 (which is threaded through the vascular system to a position so that its working head 300 is extended into the ventricle or through a coronary artery to be adjacent the site into which the flowable material will be introduced into the myocardium), the instrument 200 is arranged to penetrate the myocardium directly from the epicardium to introduce the flowable agent.

As best seen in Fig. 7 the delivery instrument 200 basically consists of two main portions, namely, a flowable agent capsule receiving portion 202 and an elongated injector tip portion 204. The capsule receiver portion 202 is in the form of an elongated body which is particularly suited to be grasped in the hand of the user. The body forms the proximal end of the instrument 200. The injector tip portion 204 is an elongated, small diameter, e.g., 1 mm, member which extends from the distal end of the body portion 202 to thereby form the distal end of the instrument. The receiver portion 202 is a generally hollow member having a cavity 206 for receipt of a rupturable capsule, like capsule 72 described heretofore. The outlet of the capsule 72 is in communication with a passageway 208 in the form of a metal tube of small bore, e.g., 0.015 inch, which extends down through the injector tip 204 to the distal end 210 thereof. As can be seen, the distal end of the tip is pointed to form a piercing member. A plurality of outlet ports 212 are provided in the distal tip and are in fluid communication with the passageway 208. The ports are equidistantly spaced about the periphery of the tip and are directed radially outward therefrom. The ports are arranged to allow the flowable agent(s) 24

to exit the instrument 200 in the form of plural, radially outwardly directed, high pressure fluid jets which are shown graphically by the arrows 24 in Fig. 7.

The delivery instrument 200 illustrated in Fig. 7 only shows the flowable agent(s) 24 delivered to the myocardium 3 in one area. However, it should be appreciated that the instrument may be positioned at different levels in the myocardium to deliver the flowable agent(s) into the entire depth of the myocardium. Further still, the distal portion 204 of the instrument 200 may include a plurality of ports 212 at different longitudinal positions therealong to distribute the flowable agent(s) into the myocardium at various levels with a single delivery or penetration.

In order to propel the flowable agent(s) out of the capsule to form those jets, the instrument 200 includes a fast acting plunger assembly. In particular, the assembly comprises a plunger 214 located immediately proximally of the piston 64 at the proximal end of the capsule 72. The plunger is located within a bore 216 in the body portion 202. A powerful spring, not shown, forming a portion of the plunger assembly is located proximally of the plunger and is normally held in a retracted, loaded position by a trigger mechanism, not shown. When the trigger mechanism is actuated by the user, it releases the spring to advance the plunger rapidly through the bore in the distal direction to engage and move the piston distally. The rapid distal movement of the piston pressurizes the agent 24 within the capsule to cause the capsule wall to burst and thereby enable the flowable agent to flow down the passageway 208 to the ports 212 where it exits in plurally radially directed high pressure jets.

It should be pointed out that the delivery instrument 200 can be constructed in accordance with the teachings of United States Letters Patent No. 2,398,544 (Lockhart) or any other prior art injector device using springs or other mechanisms for driving an agent from a capsule or receiver located therein.

In any case, the sizing of the parts of the instrument is preferably selected so that pressures of several thousand psi can be generated by the actuating mechanism, e.g., plunger and capsule combination. Such pressures are more than adequate to drive the flowable agent(s) jets a significant distance into the penetrated tissue, e.g., the myocardium.

To expedite the vascularization of cardiac tissue, the tip 210 of the device 200 is preferably pointed so that it may penetrate into the cardiac tissue a limited distance, e.g., 1 - 20 mm, such as shown in Fig. 7. Once it is at the appropriate depth, the agent 24 may then be

pressurized and forced into the tissue through the ports 212 as described earlier. Depending on the application, one or plural penetrations can be undertaken.

In some applications, a depth control means (to be described later) may be provided to limit the depth of penetration of the distal or working end of the instrument 200 into the myocardium to disperse the flowable agent(s) into the contiguous tissue. Such depth control means may comprise means to limit the depth of the lumen(s) created by the delivery instrument, or may comprise means on an insert (to be described later) which is implanted into the targeted tissue to limit its depth of penetration into the lumen or may be a combination of both. The depth control means of the delivery instrument may be adjustable to vary the depth of the lumen(s) created by the instrument. The optimal lumen depth created by the instrument may be determined before the procedure or during the procedure by measuring the thickness of the cardiac tissue with a transesophageal echocardiogram probe, ultrasound probe, or other measuring instrument.

It should be pointed out at this juncture that while the delivery instrument 200 is shown making use of a rupturable capsule 72, like that described heretofore, it should be clear that the instrument can make use of other types of capsules, such as the needle-puncturable capsule 52 described earlier, for holding the flowable agent(s). In such an alternative arrangement, a piercing needle 60, like that described heretofore, is provided in the injector located proximally of and in communication with the metal tube 208. The needle is directed towards the cavity holding the capsule so that it can pierce the end wall of the capsule when the capsule is moved into the point of the needle by the distal movement of the piston 64.

It should also be pointed out at this juncture that the flowable agent can include a flowable carrier material if desired. The flowable carrier material can be arranged to harden slightly after placement, like epoxy or silicon caulking material, so that it is not extruded from the cardiac tissue after penetration during the cardiac contraction cycle. As will be discussed later, a significant feature of the subject invention is the stimulation of a foreign body reaction and healing response in the myocardium which results in the formation of capillaries at the site of and adjacent the implanted flowable agents.

Fig. 9 is an illustration of the heart of a living human being, partially in section, showing one embodiment of another flowable agent(s) delivery instrument 400 forming a portion of a targeted tissue treatment, e.g., myocardial revascularization, system of the subject invention. In this case, the instrument is a vibratory device which is used to penetrate a portion of the

epicardium 2 and then into the myocardium 3 to deliver the flowable agent(s) into the myocardium. Vibratory energy provided by this embodiment may be sonic, ultrasonic or other energy used to create channels or lumens in the targeted tissue into which the flowable agent(s) 24 will be ejected or deposited for dispersion into tissue contiguous with the lumen or channel into which it is introduced. Alternatively, the deployment instrument 400 can provide one or more of various other types of energy to the targeted tissue to create the channels or lumens and then deliver the flowable agents therein. Examples of other types of energy contemplated for such procedure are thermal energy, mechanical energy (e.g., rotational cutting or boring, slicing, etc.), electrical energy (e.g., radiofrequency energy, etc.), hydraulic energy (e.g., pneumatic energy, radiation energy, laser or other light energy, or other types of electromagnetic energy, etc.) It should be pointed out at this juncture that the application of energy to the cardiac tissue will not only serve to create the lumens or channels but can also disable or denervate local nerves in the targeted tissue. This factor may prove particularly significant for cardiac tissue treatment applications by minimizing or otherwise reducing patient-pain resulting from angina.

In some applications, such as where the deployment instrument 400 applies electrical energy to the cardiac tissue to form the lumens or where the formations of the lumens and/or the deployment of the flowable agents therein is best accomplished during a particular portion of the cardiac cycle, the targeted tissue treatment system utilizing a vibratory instrument like instrument 400 may also include some control and sensing means (such as will be described later) that synchronizes the operation of the delivery instrument to a specific portion of the cardiac cycle.

The instrument 400 as shown herein is merely exemplary. Thus, it can be of any suitable construction. For example, it can be constructed similarly to the device disclosed in United States Letters Patent No. 4,315,742 (Sertich) whose disclosure is incorporated by reference herein. That device basically comprises an air-powered vibratory instrument which vibrates at approximately 7 KHz. This example is not intended to exclude other means for generating vibratory energy for the instrument 400, such as magnetostrictive or piezoelectric devices. In the exemplary embodiment 400 shown herein, the device basically comprises the device of the aforementioned Sertich patent with an alternative tip 402 constructed in accordance with this invention and as shown in Fig. 10 herein. In particular, as can be seen in Fig. 10, the tip 402 is an elongated angled member which is arranged to be attached to the screw thread at the distal end of the Sertich device. The angled tip is present within a holder 404. The

free end of the tip is rounded at its distal end 406 and includes plural small radially directed outlet ports 408 for distribution of the flowable agent(s) 24. The tip may be of a continuous tapered form (not shown) or a step form having a reduced diameter distal section 410 including the free end 406 as shown in the illustration of Fig. 10. The fact that the distal end of the tip is of reduced diameter coupled with the fact that it is located a distance from the holder 84 serves to amplify the vibration produced by the instrument during operation. The flowable agent 24 is provided by the instrument 400, as will be described later, and exits from the plural ports 408 in the form of plural radially directed outward jets as shown by the arrows in Fig. 9.

Fig. 11 shows a complete targeted tissue treatment system 20 making use of the vibratory delivery instrument 400 just described to effect the vascularization of the myocardium. Thus, as can be seen, the free end 406 of the tip 402 of the instrument 400 is placed against the epicardium and the foot control switch 114 is depressed to the first position. Nitrogen gas passes through the tube 110 directly to the instrument 400 thus generating vibrations in the tip 402. Concurrently, saline flows from the bag 116 through the pump 112 to the input 106B of the highest wins valve 106 and from there through the feed line 108 into the interior of the instrument 400. The saline flows through the instrument to the tip and out through the ports 408. This action bores a channel or lumen through the epicardium into the myocardium. When this has been accomplished, the foot switch is then depressed to the second position, whereupon the capsule injector ram 68 of the system 20 is driven smartly into the capsule 52, thereby ejecting the flowable agent(s) 24 through the highest wins valve port 106A into the feed tube 108. The agent(s) 24 is delivered through the instrument 404 to its tip 402 either by continued motion of the injector (assuming the capsule charge is large enough) or carried forward by the continuing flow of saline from the pump. The flowable agent thus is driven into the myocardium by the use of pressure alone or by the vibration of the instrument alone or by a combination of both.

Fig. 12 is an illustration, not to scale, of the heart of a living human being, shown partially in section, and illustrating an embodiment of another alternative flowable agent(s) delivery instrument (not to scale) forming a portion of a targeted tissue, e.g., myocardial revascularization, system of the subject invention. This embodiment is denoted by the reference number 500 and basically comprises a jet injector which is used to deliver the flowable agent(s) 24 as a pressurized stream into the myocardium 3 via the epicardium 2.

As is known, pressurized fluids have been used in the past in jet injector devices for administering intramuscular and subcutaneous medications to a patient through the patient's skin, without the use of a skin-penetrating needle. The advantages of such systems include the reduction of pain and apprehension associated with needle injections, the elimination of needle-stick injuries, and the reduction of environmental contamination associated with needles. Jet injection devices have been considered for immunization vaccines, hormone delivery, local anesthetics, and insulin delivery. For example, United States Letters Patent No. 2,398,544 (Lockhart) discloses a hypodermic injector for administering a liquid through the skin of a living being without the necessity of having a needle puncture the skin. The device uses a pressure of 8,000 to 10,000 psi to force a stream of a liquid through the skin. United States Letters Patent No. 2,737,946 (Hein) discloses an apparatus for hypodermically injecting medicants through the skin without the use of a penetrating needle. United States Letters Patent No. 2,762,370 (Venditty) discloses a needleless hypodermic injector for use in discharging liquid medicants from an orificed ampule in the form of a minute stream. An initial high-pressure discharge causes the jet stream to distend the skin and force the liquid to a predetermined depth beneath the surface. After the minute opening in the epidermis has been produced, the pressure of the stream is immediately reduced to a lower second stage for completing transfer of the remaining liquid from the ampule. United States Letters Patent No. 2,800,903 (Smoot) discloses a device for the injection of a medicant without the use of a long needle. United States Letters Patent No. 5,704,911 (Parsons) discloses a system utilizing hypodermic jet injections to deliver liquid medicants without piercing the skin with a needle. United States Letters Patent Nos. 4,165,739 (Doherty et al.) and 3,815,514 (Doherty) disclose inoculators for injecting a fluid through the skin without the use of a needle.

Referring now to Fig. 12, it can be seen that the jet injector delivery instrument 500 as illustrated is constructed similarly to the inoculation injector described in United States Letters Patent No. 2,398,544 (Lockhart) whose disclosure is incorporated by reference herein. This construction is referred to since it is illustrative of some forms of devices that are suitable for the purpose of injecting a flowable agent into a targeted tissue, e.g., the myocardium, under high pressure. Other types of jet injectors could be utilized in accordance with this invention.

As can be seen clearly in Fig. 12, a capsule 502 containing a flowable agent(s) constructed in accordance with this invention is held within a dispensing chamber in a cap portion 504 of the jet injector instrument 500. The cap includes multiple tiny orifices 506

arranged in a pattern, e.g., equidistantly spaced and slightly flared outward, to give a wide spread to the injected agent(s) 24 within the myocardium. Alternatively, the injector device may only include a single orifice for injecting a single jet stream of the agent into the myocardium. In the embodiment shown, the instrument 500 includes an activatable plunger 508 which is arranged to be released by axial motion of a sleeve 510 to rapidly engage or push into the capsule 502. This action propels the flowable agent(s) 24 of the capsule through the orifices 506 in the cap 504 and into the contiguous cardiac tissue, i.e., through the epicardium and into the myocardium as shown by the arrows in Fig. 12.

It should be pointed out at this juncture that the instrument 500 may be constructed differently. For example, the instrument 500 could consist of a local jet holder, like cap 504, but with the pressure source and capsule remote from the tip.

During the operation of the system of Fig. 12, the agent or carrier fluid for the agent (to be described later) intended for introduction into the targeted tissue is inserted in a proper dosage into the dispensing chamber. As discussed previously, pre-dosed capsules can be utilized. In any case, the plunger is driven forward by the linearly applied force and converts this force into pressure on the flowable agents. The force is sufficient to cause the flowable agents to exit the chamber via the orifice(s) 506 at such a velocity that they can be hypodermically injected into the injection site. It is possible that an ampule or other agent reservoir could be used and as such the ampule could utilize a dosage scale or graduations for use in metering proper doses. Moreover, it is conceived, but not illustrated, that an embodiment of a needleless hypodermic injection delivery instrument of this invention would include an ampule assembly having a chamber for holding the flowable agent(s), e.g., a liquid suspension, and an injector for receiving and mounting the ampule assembly. In such a case, the ampule assembly will have an opening at an end of an ampule shell through which the flowable agent can be drawn into and ejected out from. A plunger assembly movable within the chamber is used for drawing the flowable agent into the chamber and for injecting the material out of the chamber. The injector applies a force that activates a plunger to thereby force the material to leave the chamber via the orifice(s) at a velocity sufficient that the agent can be hypodermically injected into the targeted tissue. The force may be applied by a firing mechanism that releases compressed gas from a storage compartment. The compressed gas acts upon a piston which drives the plunger to subsequently eject the preselected dosage of the flowable agent(s) through the orifice(s) at the distal end of the instrument. A shock absorber may be used to soften or

cushion the shock of the triggering mechanism. For some flowable agents, e.g., vaccines, there may be a standard implant dosage, while for other agents there may be variable size dosages, e.g., weight dependent medications. Safety interlocks, not shown, can be incorporated to prevent system activation until the delivery instrument is fully secured in position.

In some applications it may be desirable to stabilize the flowable agent(s) delivery instrument against the targeted tissue, e.g., the endocardium or epicardium during the tissue treatment, e.g., revascularization, procedure. For such applications, the system 20 may make use of some releasable securement or attachment means, like that shown in Fig. 13. That means basically comprises a suction hood, to be described in detail later, which stabilizes or otherwise holds the flowable agent delivery instrument in place. Once positioned, the delivery instrument can be activated to direct the flowable agent(s) therefrom into the targeted tissue. It must be pointed out at this juncture that the use of the stabilization as disclosed herein is not confined to the use with any particular type of delivery instrument. Thus, it can be used with powered, e.g., rotatable working head instruments like shown in Fig. 2, or manually driven instruments like shown in Figs. 7, 9 and 13, to create lumens within the targeted tissue and to introduce the flowable agent(s) therein. Fig. 13 illustrates one such device when applied to the delivery instrument of Fig. 7. Thus, referring now to Fig. 13, there is shown a delivery instrument 200 of Fig. 7 but including a releasably securable attachment mechanism 600 in the form of a suction hood 602 assembly and associated components. The suction hood assembly is slidably mounted on the distal portion 204 of the instrument 200. The suction hood assembly 602 basically comprises a cup-shaped hollow member formed of a resilient material, e.g., silicone rubber, having a central passageway 604 therein for accommodating the distal end portion 204 of the delivery instrument 200 (or any other delivery instrument). The periphery of the cup-shaped member is in the form of an enlarged flange which is arranged to directly engage the epicardium or other targeted tissue. A source of vacuum 606 is provided coupled to the proximal end of a tube 608 in communication with the interior of the cup-shaped hood. The vacuum source 606 is arranged to be actuated by the operator of the system via any suitable means (not shown). This action couples the vacuum source 606 to the interior 610 of the hood to produce suction at the distal end of the hood thereby holding it in place on the targeted tissue, e.g., epicardium, centered over the location at which the delivery instrument 200 is to enter the underlying tissue. The operator can then drive the instrument 200 inwardly into and through the epicardium and into the myocardium with the suction cup stabilizing the zone of interest.



Fig. 14 shows the flowable agent(s) delivery device 300 of Fig. 8 but used in a tissue treatment application wherein the distal end portion of the instrument is fed through the urethra 14 into the prostate gland 15 of a living male being for the purpose of delivering the flowable agent(s) 24 into the prostate gland in the form of jets of that agent. The instrument 200 could thus be used to treat prostate cancer, benign prostate hyperplasia, or other prostate conditions with suitable flowable treatment agent(s), such as tissue and/or vascular antagonists. If desired, the instrument may be positioned so that its distal end is within the bladder 16 to deliver the flowable treatment agent(s) thereto for treating a tumor T.

In accordance with one preferred aspect of this invention, the flowable agent(s) is in the form of a plurality, e.g., a host or myriad, of small particles of one or more materials (the materials to be described in the tables to follow) either alone or in combination with some carrier fluid, e.g., a liquid. Preferably, the particles are in the form of microspheres or other microparticles. Figs. 15A-15H show respective embodiments of the microparticles which may be used as the flowable agent or as part of the flowable agent or for delivering flowable agents into the tissue of a living being in accordance with this invention.

As described previously, the agents 24 are formed of at least one material that can elicit a beneficial response within cardiac or other tissues. For example, the agents can be of a pharmaceutical or genetic nature and their presence can initiate a bio-chemical/biological process that stimulates the tissue to heal itself. The agents can also trigger the onset of a foreign body or healing response to cause the formation of lumens in communication with the arterial system.

Before describing the exemplary embodiments of the microspheres shown in Figs. 15A-15I

The flowable materials may be of any particulate size from approximately 1 micron to approximately 1 mm. In Figs. 15A-15I, the particles are shown as being microspheres or microparticles.

Referring now to Fig. 15A, it can be seen that while there is shown a single microsphere 700 which along with others can be used to form the flowable agent. The microsphere 700 basically comprises an outer layer 702 and an inner core 704. The outer and inner layers may be of different materials or contain different agents or different concentrations of the same agent. By varying the absorption rate of the different layers, the release rate of any agent stored

in the material will vary accordingly. Additionally, the inner core can be an encapsulated liquid containing an agent or plural agents.

Fig. 15B shows a microsphere 706 having a matrix of small pockets of agents 708 dispersed therein. As the microsphere 706 is absorbed, the agents in the matrix are released.

Fig. 15C shows a microsphere 710 having a matrix of small pockets of agents 714 dispersed therein and which matrix is coated by a continuous shell 714. The shell can contain no agent or different agents than are contained in the interior matrix.

Fig. 15D shows a microsphere 716 having an outer layer 718 and an encapsulated liquid core 719 containing the agent(s).

Fig. 15E shows a microsphere 720 having multiple layers 722 with thin coatings of agents 724 between each layer. As the layers 722 are absorbed, the agents 724 between the layers will be released. Additionally, the thin layers may comprise a material that may not be related to the treatment of the targeted tissue; but rather is an intermediate material which connects two layers of material. For example, it may comprise a coating applied to a polymer surface that contains receptors for a specific biological material, e.g., a recombinant adenovirus expressing human fibroblast growth factor-2 (FGF-2).

Fig. 15F shows a homogeneous microsphere 726 that is evenly seeded with agents 728 throughout. The agents 728 are uniformly released as the microsphere is absorbed.

Fig. 15G shows a microsphere 730 that is coated with a thrombogenic agent 732 such as thrombin, that will promote clotting of blood around the agent to prohibit movement of the agent through the tissue after it is deposited.

Fig. 15H shows a microparticle (not a sphere, but rather an irregularly shaped body) 734 seeded with a matrix of encapsulated agents 736 throughout. The irregular shape of the body 734 tends to render it resistant to movement after it is deposited in the targeted tissue.

Fig. 15I shows a small shard or piece of a polymer 738 or some other material that could be coated or seeded with a suitable treatment agent. The irregular shape of the polymer body also serves to prevent movement of it after it is deposited in the targeted tissue.

As is known, microspheres are well known for their use in long term controlled release of drugs or other therapeutic agents. This is a highly developed technology that has been used in many applications and such microspheres are available from a variety of sources (e.g., Polymicrospheres, Indianapolis, IN). The microsphere structures typically consists of: (a) a continuous drug phase surrounded by a continuous barrier membrane or shell (microcapsule),

(b) a shell structure where the drug phase is subdivided into numerous domains scattered uniformly through the interior of the microsphere, (c) a polymer matrix throughout which the drug is uniformly dispersed, (d) a structure where the drug is either dissolve or molecularly dispersed within the carrier material from which the microsphere is prepared, and (e) solid. The most common method of delivering drugs or other therapeutic agents with microspheres incorporates these agents uniformly within a polymer matrix.

The fabrication of and application of microspheres is well known and as such the following examples are included herein as reference. United States Letters Patent No. 3,887,699 describes a solid biodegradable polymer spheroids implants which incorporate a drug for sustained release as the polymer naturally degrades in the human body. Many different methods of constructing this type of controlled release system have been developed. Although the uniform matrix of a polymer provides a simple and efficient means of controlled release of agents with microspheres, many advanced methods of containing and releasing the therapeutic agents have been developed. United States Letters Patent No. 4,637,905 (Gardner) discloses a method for encapsulating a therapeutic agent within a biodegradable polymer microsphere. United States Letters Patent No. 4,652,441 (Okada et al.) discloses a method of utilizing a water-in-oil emulsion to give prolonged release of a water-soluble drug. The patent describes a wide variety of drugs that can be delivered via prolonged release micro-capsules as well as suitable polymeric materials and drug retaining substances. It is conceived that the system of this invention could incorporate any of the drugs described to in this patent to generate a beneficial effect in the cardiac tissue. United States Letters Patent No. 5,718,921 (Mathiowitz et al.) discloses a method for constructing a multiple layer microsphere which can release two different drugs at controlled rates or a single drug at two different rates. United States Letters Patent No. 5,912,017 (Mathiowitz et al.) also discloses a method of forming two layered microspheres by using an organic solvent or melting two different polymers, combining them with a desired substance and cooling. Microspheres are not limited to just water-soluble therapeutic agents. See, for example, United States Letters Patent No. 5,288,502 (McGinity et al.) which discloses a multi-phase microsphere which is capable of incorporating water-soluble and water-insoluble drugs.

Several embodiments of the subject invention utilize the incorporation of therapeutic agents into microparticles or microspheres that degrade over time and release the therapeutic agents. As a non limiting example, microparticles can be used to deliver any type of molecular

compound, such as proteins, genetic materials, proteins, peptides, pharmacological materials, vitamins, sedatives, steroids, hypnotics, antibiotics, chemotherapeutic agents, prostaglandins, and radiopharmaceuticals. The delivery system of the present invention is suitable for delivery the above materials and others including but not limited to proteins, peptides, nucleotides, carbohydrates, simple sugars, steroids, pharmaceuticals, cells, genes, anti-thrombotics, anti-metabolics, growth factor inhibitor, growth promoters, anticoagulants, antimetotics, and antibiotics, fibrinolytic, anti-inflammatory steroids, and monoclonal antibodies. Examples of deliverable compounds are listed in Table 1 and 2.

**Table 1: Examples of Biological Active Ingredients**

Growth factors  
Genetic material  
Fibroblast Growth Factor (FGF)  
Adenovirus  
Bone morphogenic proteins (BMP)  
Hormones  
Stem Cells  
Vascular Endothelial Growth Factor (VEGF)  
Interlukins  
Insulin-like Growth Factors (e.g. IGF-I)  
Platelet-derived Growth Factor (PDGF)

**Table 2: Examples of Pharmaceutical ingredients**

Thrombin  
Anti-inflammatorys  
Anti-proliferative agents  
Immunosuppressant agents  
Glycosaminoglycans  
Collagen inhibitors  
Anticoagulants  
Anti-bacterial agents  
Vasodilators  
Calcium channel blockers

ACE inhibitors

Beta blockers

Antiarrhythmics

Antiplatelets

Thrombolytics

Microspheres can be made of a variety of materials such as polymers, silicone and metals. Biodegradable polymers are ideal for use in creating microspheres. There are essentially three classes of biodegradable polymers: (1) water-soluble polymers rendered insoluble by hydrolytically unstable cross-linking agents, (2) water-insoluble polymers that become soluble by hydrolysis but retain their molecular backbone, and (3) water-insoluble polymers that become soluble by backbone cleavage. Polylactic Acid and Polyglycolic Acid are well known examples of resorbable polymers. The release of agents from absorbable microparticles is dependent upon diffusion through the microsphere polymer, polymer degradation and the microsphere structure. Although most any biocompatible polymer could be adapted for this invention, the preferred material would exhibit in vivo degradation. It is well known that there can be different mechanisms involved in implant degradation like hydrolysis, enzyme mediated degradation, and bulk or surface erosion. These mechanisms can alone or combined influence the host response by determining the amount and character of the degradation product that is released from the implant. The most predominant mechanism of in vivo degradation of synthetic biomedical polymers like polyesters, polyamides and polyurethanes, is generally considered to be hydrolysis, resulting in ester bond scission and chain disruption. In the extracellular fluids of the living tissue, the accessibility of water to the hydrolysable chemical bonds makes hydrophilic polymers (i.e. polymers that take up significant amounts of water) susceptible to hydrolytic cleavage or bulk erosion. Several variables can influence the mechanism and kinetics of polymer degradation. Material properties like crystallinity, molecular weight, additives, polymer surface morphology, and environmental conditions. As such, to the extent that each of these characteristics can be adjusted or modified, the performance of this invention can be altered.

Finally, many biodegradable polymers are also used to construct these microspheres such as polylactide, polyglycolide, copolymers with glycolides, lactides and/or epsilon-caprolactone, polyanhydrides, polyorthoesters, and many others. The polymers of poly (D,L-lactic acid) and poly (D,L-lactic) co-glycolic acid are among the most preferred polymers used

historically for controlled release. However, virtually any biodegradable and/or biocompatible material may be used with the present invention. A list of example biocompatible materials are shown in Tables 3 and 4.

**Table 3: Biodegradable Polymer Examples**

Polyglycolide (PGA)  
Polylactide  
Copolymers of glycolide  
Glycolide/L-lactide copolymers (PGA/PLLA)  
Glycolide/trimethylene carbonate copolymers (PGA/TMC)  
Polylactides (PLA)  
Poly-L-lactide (PLLA)  
Poly-DL-lactide (PDLLA)  
L-lactide/DL-lactide copolymers  
Lactide/tetramethylglycolide copolymers  
Lactide/trimethylene carbonate copolymers  
Lactide/ $\sigma$ -valerolactone copolymers  
Lactide/ $\epsilon$ -caprolactone copolymers  
Polydepsipeptides  
PLA/polyethylene oxide copolymers  
Poly- $\beta$ -hydroxybutyrate (PBA)  
PHBA/ $\gamma$ -hydroxyvalerate copolymers (PHBA/HVA)  
Poly- $\beta$ -hydroxypropionate (PHPA)  
Poly-p-dioxanone (PDS)  
Poly- $\sigma$ -valerolactone  
Poly- $\epsilon$ -caprolactone  
Methyl methacrylate-N-vinyl pyrrolidone copolymers  
Polyesteramides  
Polyesters of oxalic acid  
Polydihydropyrans

Polyalkyl-2-cyanoacrylates  
Polyurethanes (PU)  
Polyvinyl alcohol (PVA)  
Polypeptides  
Poly- $\beta$ - malic acid (PMLA)  
Poly- $\beta$ - alkanolic acids  
Trimethylene carbonate  
Polyanhydrides  
Polyorthoesters  
Polyphosphazenes  
Poly (trimethylene carbonates)  
PLA-polyethylene oxide (PELA)  
Tyrosine based polymers

**Table 4: Examples of other suitable materials**

Alginate  
Calcium  
Calcium Phosphate  
Ceramics  
Cyanoacrylate  
Collagen  
Dacron  
Elastin  
Fibrin  
Gelatin  
Glass  
Gold  
Hydrogels  
Hydroxy apatite  
Hydroxyethyl methacrylate  
Hyaluronic Acid

Liposomes  
Nitinol  
Oxidized regenerated cellulose  
Phosphate glasses  
Polyethylene glycol  
Polyester  
Polysaccharides  
Polyvinyl alcohol  
Platelets, blood cells  
Radiopaque  
Salts  
Silicone  
Silk  
Steel (e.g. Stainless Steel)  
Synthetic polymers  
Thrombin  
Titanium

It must be pointed out at this juncture that the agents of this invention are preferably configured such that their presence in the myocardial tissue does not significantly limit the contractility of the cardiac muscle. As previously described, the agents may be coated with or contain growth factors, anti-oxidants, seeded cells, or other drug/biologically active components depending upon the result desired.

The main feature of these constructions is to stimulate a foreign body reaction and a healing response which results in the formation of capillaries at the site of the implant. Moreover, the angiogenesis action resulting by the location of the agents within the lumens over time will further revascularize the myocardium. As such, these implants may provide less of a short term improvement to vascularization, but instead will lead to a long term improvement.

As should be appreciated from the foregoing whether the system 20 makes use of non-resorbable or resorbable agents is of little relevance from the standpoint of increased blood flow to the myocardium tissue and capillaries contiguous with the lumens so long as the agents are constructed suitably.



Figure 16 is an illustration of a portion of the heart of a living human being, partially in section, showing the embodiment of a jet injector delivery instrument 200 (described earlier and shown in Fig. 7) shown used to deliver the flowable agent(s) of this invention into the myocardium 3 via the epicardium 2. The coronary vessels 17 perfusing the myocardium are at least partially obstructed by atherosclerotic material 18. As previously described, the device 200 utilizes a pressurized stream to distribute the flowable agents into targeted tissues. In this particular embodiment, microparticles or microspheres like those described earlier and shown in Fig. 15 are implanted or injected into a portion of myocardium in the form of a micro dispersion. The velocity of the microparticles when exiting the instrument may be of sufficient velocity to penetrate the myocardium but not penetrate a coronary vessel if encountered. As previously discussed the instrument 200 may be stabilized on the surface of the heart and the depth of the instrument in the myocardium may also be controlled. One embodiment of a stabilizing and depth control member 800 is shown as part of the instrument 200.

Referring to Figure 17, after the instrument 200 shown in Fig. 16 is removed, the microdistribution of microparticles 24 remain in the myocardium 3. The microparticles 24 are sufficiently implanted into the myocardium to resist movement. The combination of the microparticles and the injury created by the instrument 200 to deploy and disperse the particles may effect angiogenesis. Additionally a channel or lumen 19 remains in the myocardium area where the instrument was inserted. An insert or plug 802 may be placed in the channel 19 after the instrument 200 is removed. This action may assist in achieving hemostasis of the puncture. For this purpose, the insert or plug 802 may be formed of a hemostatic material, such as collagen or alginate, and may incorporate thrombogenic material, such as thrombin, to accelerate hemostasis of the channel. The insert or plug 802 may also have an enlarged proximal head portion 804 that may limit the depth of insertion depth of the insert or plug and may also serve to stabilize the insert or plug against the surface of the myocardium. The insert or plug 802 may also be formed of a material which will contribute to the improved revascularization such as those listed on Tables 3 and 4. The insert may also serve to maintain the patency of the channel or lumen. As such, a portion of the insert or plug can be perforated or include channels (see for example the inserts of the aforementioned copending application S.N. 08/958,788). The insert itself may also act to treat the surrounding tissue. For example, the insert or plug 802 may also comprise a biologically active ingredient or pharmaceutical ingredient as listed on Tables 1 and 2. Finally, the insert or plug 802 may also be useful in the

selective ablation or improvement of electrical conduction pathways, or the selective ablation or improvement of the nerves of the tissue.

Figure 18 shows the condition of the myocardium 3 after angiogenesis has occurred to create significant new vasculature, e.g., capillaries C. As can be seen at this time, the microparticles 24 and the insert 802 have been absorbed and the channel 19 formed by the instrument have healed. In addition and quite significantly, the microparticles, the insert, and any biologically active materials or pharmaceutical agents which may have also been implanted have induced the growth of the new vasculature (capillaries) C or otherwise improved the tissue.

Fig. 19 is an illustration of a portion of the heart 1 of a living being, shown partially in section and showing the embodiment of the delivery instrument 200 of Fig. 7 used to deliver the flowable agent(s) 24 into the myocardium in the form of pressurized streams of fluid. In this figure three instruments 200 are illustrated for introducing the flowable agents into the myocardium at three different locations 902, 904, and 906. While three delivery instruments 200 are illustrated extending into the myocardium together, the system 20 will typically only include a single delivery for delivering the agents to one site 902, 904 and 906 in the myocardium at a time. Therefore, it should be understood that Fig. 19 should be understood to depict the sequential delivery of the flowable agent(s) 24 into the myocardium 3 by a single delivery instrument 200.

At high pressures, the stream of flowable agent(s) 24 delivered to the myocardium may cause separation of the myocardial muscular fibers and may form a channel in the myocardium. If the delivery instrument is inserted into the myocardium at several locations at controlled distances between insertion points, the channels formed by the pressurized stream of fluid may be contiguous with one another, thus forming a long channel within the myocardium. Furthermore, a portion of the myocardium may be normally perfused with blood and an adjacent portion of the myocardium may be ischemic. If the instrument 200 is inserted in a plurality of locations at controlled distances between insertion points in the normally perfused myocardium and extending into and possibly through the ischemic myocardium, an intramyocardial channel (like that designated by reference number 908 in Fig. 20) from the normally perfused myocardium extending into the ischemic myocardium results. This channel is expected to remain patent, thereby resulting in immediate increased perfusion to the ischemic myocardium.

Regardless of the immediate patency of the channel 908, the combination of the mechanical injury produced by the creation of the channel and the flowable agents 24 may

cause the creation of additional vasculature including and in addition to the formed channel, thereby resulting in increased perfusion of the portion of ischemic myocardium. Depending on the degree of ischemia and the area of ischemic myocardium, several channels may be formed in the area of the ischemic myocardium. The channels may or may not originate or terminate in a portion of normally perfused myocardium.

Regarding the pressurized stream of fluid used to create the channel 908, the instrument 200 may utilize multiple flowable agents 24 to create the channel and implant agents into the myocardium. For example, one flowable agent, e.g., saline mixed with contract medium, may be used to create the channel and a second flowable agent, e.g., saline with bFGF coated microspheres and VEGF coated microspheres, may be implanted into the channel and at some significant distance into the myocardium surrounding the created channel. Additionally, the channel may be formed in communication with an existing coronary vessel to provide significant blood flow to the channel. The communication of existing vessel and channel may be effected by creating an opening in the existing vessel with the delivery of flowable agent in a pressurized stream from within the myocardium or from within the vessel.

Fig. 20 is an illustration of a portion of the heart shown in Fig. 19, but after its treatment by the system of the subject invention. Thus, as can be seen, the channel 908 in the myocardium which was created by the delivery system of the subject invention is open and may extend between normally perfused myocardium and ischemic myocardium to provide immediate blood flow to the ischemic myocardium. In addition or alternatively the channel 908 may serve as a means whereby new blood vessels may grow, supplemented by the introduction of a flowable agent as previously described.

In order to prevent the flow of blood from the channel 908 through the instrument's entry sites 902, 904 and 906 into the myocardium, a hemostatic insert may be applied in each channel created by the instrument, like that described with reference to Fig. 17. Alternatively, an adhesive material, e.g., fibrin glue, may be applied to the surface of the myocardium at the delivery instrument insertion point or within the channel created by the instrument, to cause the original entry channels close down as shown in Fig. 20.

Fig. 21 is an enlarged sectional view of the distal end portion of the treatment agent delivery instrument 1000 forming a portion of the tissue treatment system 20 of this invention. The delivery instrument 1000 incorporates an energy applicator, e.g., a laser (not shown), to provide energy denoted by the arrows designated by the reference numbers 1004 into the

targeted tissue, e.g., the myocardium 3, to produce a channel therein and into which the flowable agent(s) 24 may be introduced. In particular, the laser beam 1004 from the laser is carried down the instrument 1000 via any suitable laser energy conductor, e.g., a light pipe or fiber optic cable 1006. An annular passageway 1008 is provided within the distal end portion of the instrument 1000 surrounding the laser energy conductor 1006. A plurality of exit ports 1010 are located at peripherally spaced locations at the distal end of the instrument adjacent the free end at which the laser energy conductor 1006 terminates and are in fluid communication with the passageway 1008. The passageway 1008 and the communicating ports 1010 serve as the means to enable the flowable agent(s) 24 to exit from the instrument in plural jets.

The instrument 1000 of Fig. 21 is inserted into the targeted tissue, e.g., the myocardium, by applying laser energy from the laser source through the conductor 1006 so that the laser beam 1004 penetrates into the tissue to form a channel into which the distal end of the instrument 1000 may be inserted. Once the instrument 1000 is within the channel in the tissue, the flowable agent(s) 24 may be introduced into the tissue by causing it to flow down the annular passageway 1008 and out through the ports 1010 in the form of pressurized jets. The combination of the application of the energy to create the channel plus the delivery of the flowable agent(s) 24 into the tissue contiguous with the channel is expected to result in increased beneficial effects to that tissue, such as the formation of new vasculature, denervation, and ablation of electrical conduction pathways.

In Fig. 22, there is shown an alternative embodiment of a laser-energy based delivery instrument 1020. In this embodiment, the distal end of the instrument 1020 includes an annular laser energy conductor 22 for carrying the laser energy or beam 1004 down it from the laser energy source (not shown) so that the laser beam exits the instrument in a somewhat coaxial direction as shown. A central passageway 1024 is provided in the instrument located within the central opening in the annular laser conductor 1022. The passageway 1024 terminates at its distal end in a wall having plural outlet ports 1026. The ports 1026 are directed in a longitudinal or axial direction with respect to the instrument. It is through these ports 1026 that the flowable agent(s) 24 is ejected from the instrument 1020 in the form of pressurized jets as shown in Fig. 22.

It should be pointed out at this juncture that the instrument in Figs. 21 and 22 can utilize RF energy or other electromagnetic energy to produce the channels in the targeted tissue in lieu of the laser beam described. In any case with the embodiment 1000 shown in Fig. 21, the

flowable agent is ejected in a radial direction, whereas with the embodiment of 1020 of Fig. 22, the flowable agents are ejected in an axial direction.

It should also be pointed out that the tissue treatment systems of this invention may be used without the inclusion of particles in the flowable agent. In such a case a fluid, e.g., a liquid or gas, fluid without particles but which may contain one or more of biologically active or pharmaceutical agents, such as but not limited to the agents disclosed in Tables 1 and 2 is delivered into the targeted tissue. Furthermore, the system described herein for the treatment of cardiac tissue may also be used in other tissues in the body to effect similar beneficial treatment. For example, constriction of peripheral arteries often creates areas of ischemic tissue not unlike ischemic myocardium as a result of coronary artery disease. The system of this invention may be used in these or other tissues to deliver therapeutic agents to improve blood flow through the creation of new vasculature. Other beneficial effects on the targeted tissue which may be achieved by the subject invention are pain reduction resulting from denervation in the treated tissue and interruption of electrical conduction pathways in the treated tissue resulting from ablation or some other process.

Without further elaboration the foregoing will so fully illustrate our invention that others may, by applying current or future knowledge, adopt the same for use under various conditions of service.

**CLAIMS**

1. A system for vascularizing the cardiac tissue of a living being to cause the formation of lumens in communication with the being's arterial system, said system comprising a delivery instrument and a flowable agent, said flowable agent comprising a plurality of small particles for introduction into the cardiac tissue, said delivery instrument being arranged to introduce said flowable agent at or adjacent the cardiac tissue by imparting a force to said agent, whereupon said agent directly enters the cardiac tissue at an entry situs.
2. The system of Claim 1 wherein at least some portion of some of said particles being formed of a material to cause the formation of lumens in communication with the being's arterial system.
3. A system for treating cardiac tissue of a living being to affect the conduction of electrical signals in the cardiac tissue, said system comprising a delivery instrument and a flowable agent, said flowable agent comprising a plurality of small particles for introduction into the cardiac tissue, said delivery instrument being arranged to introduce said flowable agent at or adjacent the cardiac tissue by imparting a force to said agent, whereupon said agent directly enters the cardiac tissue at an entry situs.
4. The system of Claim 3 wherein at least some portion of some of said particles being formed of a material to affect the conduction of electrical signals in the cardiac tissue.
5. A system for treating cardiac tissue of a living being to affect the conduction of nerve signals in the cardiac tissue, said system comprising a delivery instrument and a flowable agent, said flowable agent comprising a plurality of small particles for introduction into the cardiac tissue, said delivery instrument being arranged to introduce said flowable agent at or adjacent the cardiac tissue by imparting a force to said agent, whereupon said agent directly enters the cardiac tissue at an entry situs.
6. The system of Claim 4 wherein at least some portion of some of said particles being formed of a material to affect the conduction of nerve signals in the cardiac tissue.
7. The system of any of Claims 1, 3 and 5 wherein said system is arranged so that when said agent is introduced into the entry situs said agent disperses into adjacent cardiac tissue for confinement therein.
8. The system of Claim 7 where said agent comprises a material rendering said particles resistant to further dispersion into the body of the being.

9. The system of any of Claims 1, 3 and 5 wherein said delivery instrument comprises a rotary head for imparting said force to said agent.

10. The system of any of Claims 1, 3 and 5 wherein said delivery instrument comprises a fluid jet for imparting said force to said agent.

11. The system of Claim 10 wherein said delivery instrument has a distal end portion at which said fluid jet is located and a piercing tip adjacent said fluid jet.

12. The system of any of Claims 1, 3 and 5 wherein said delivery instrument comprises an elongated flexible member arranged for insertion through at least a portion of the vascular system of the being.

13. The system of Claim 9 wherein said delivery instrument comprises an elongated flexible member arranged for insertion through at least a portion of the vascular system of the being.

14. The system of Claim 10 wherein said delivery instrument comprises an elongated flexible member arranged for insertion through at least a portion of the vascular system of the being.

15. The system of any of Claims 1, 3 or 5 wherein said instrument is arranged for dispensing a controlled volume of said agent into the cardiac tissue.

16. The system of any of Claims 2, 4 or 6 wherein said at least some portion of at least some of said particles of said agent comprise material for eliciting a foreign body or healing response by the cardiac tissue.

17. The system of any of Claims 2, 4 or 6 wherein said at least some portion of at least some of said particles of said agent comprise material for eliciting a beneficial response by the cardiac tissue.

18. The system of any of Claims 1, 3 or 5 wherein said system includes means to limit the depth of penetration of said particles into the cardiac tissue.

19. The system of any of Claims 1, 3 or 5 wherein said instrument is arranged to be inserted into the interior of the heart to introduce said agent into the myocardium via the endocardium.

20. The system of any of Claims 1, 3 or 5 wherein said instrument is arranged to be inserted into the vascular system of the being to introduce said agent into the cardiac tissue.

21. The system of any of Claims 1, 3 or 5 wherein said instrument is arranged to be inserted into the vascular system of the being to introduce said agent into the myocardium via a coronary artery.

22. The system of any of Claims 1, 3 or 5 wherein said instrument is arranged to be inserted into the chest cavity of the being to introduce said agent into the wall of the myocardium via the epicardium.

23. The system of any of Claims 1, 3 or 5 wherein said system includes piercing means for producing channels in the myocardium.

24. The system of Claim 23 wherein said instrument is arranged to deploy said agent into respective ones of the channels after the formation thereof.

25. The system of any of Claims 1, 3 or 5 wherein said system applies energy to the myocardium to treat the cardiac tissue.

26. The system of Claim 20 wherein said system applies energy to the myocardium to produce channels therein.

27. The system of Claim 20 wherein said energy is selected from the group consisting of one or more of mechanical, electrical, thermal, electromagnetic, optical, vibratory, hydraulic, pneumatic, and nuclear energy.

28. The system of Claim 23 wherein said piercing means comprises means for applying a biologically active material to the myocardium to result in the production of the channels.

29. The system of any of Claims 1, 3 or 5 additionally comprising means for monitoring the cardiac cycle of the being and for coordinating the operation of said instrument with the cardiac cycle.

30. The system of any of Claims 1, 3 or 5 wherein said system additionally comprises stabilizing means for stabilizing the position of said instrument adjacent the cardiac tissue during the introduction of said agent in the cardiac tissue.

31. The system of any of Claims 2, 4 or 6 wherein said at least some portion of at least some of said particles of said agent comprises one or more of the group consisting of pharmaceuticals, biologically active materials, growth factors, radioactive materials, and radiopaque materials.

32. The system of any of Claims 2, 4 or 6 wherein said at least some portion of at least some of said particles of said agent are formed of a resorbable material.



33. The system of any of Claims 2, 4 or 6 wherein said at least some portion of at least some of said particles of said agent are microspheres.

34. The system of Claim 31 wherein said group comprises biologically active materials consisting of growth factors, genetic materials, fibroblast growth factors (FGF), Adenovirus, bone morphogenic proteins (BMP), hormones, stem cells, vascular endothelial growth factors (VEGF), Interlukins, Insulin-like growth factors (e.g., IGF-I), platelet-derived growth factors (PDGF), and tissue and/or vascular antagonists.

35. The system of Claim 31 wherein said group comprises pharmaceuticals consisting of thrombin, anti-inflammatories, anti-proliferative agents, immunosuppressant agents, Glycosaminoglycans, collagen inhibitors, anticoagulants, anti-bacterial agents, Vasodilators, calcium channel blockers, ACE inhibitors, beta blockers, Antiarrhythmics, Antiplatelets, and Thrombolytics.

36. The system of any of Claims 1, 3 or 5 wherein said at least some portion of at least some of said particles of said agent are selected from the group of biodegradable polymers consisting of polyglycolide (PGA), polylactide, copolymers of glycolide, glycolide/L-lactide copolymers (PGA/PLLA), glycolide/trimethylene carbonate copolymers (PGA/TMC), Polylactides (PLA), poly-L-lactide (PLLA), poly-DL-lactide (PDLA), L-lactide/DL-lactide copolymers, lactide/tetramethylglycolide copolymers, lactide/trimethylene carbonate copolymers, lactide/ $\sigma$ -valerolactone copolymers, lactide/ $\epsilon$ -caprolactone copolymers, Polydepsipeptides, PLA/polyethylene oxide copolymers, Poly- $\beta$ -hydroxybutyrate (PBA), PHBA/ $\gamma$ -hydroxyvalerate copolymers (PHBA/HVA), poly- $\beta$ -hydroxypropionate (PHPA), poly-p-dioxanone (PDS), poly- $\sigma$ -valerolactone, poly- $\epsilon$ -caprolactone, Methyl methacrylate-N-vinyl pyrrolidone copolymers, polyesteramides, polyesters of oxalic acid, polydihydropyrans, polyalkyl-2-cyanoacrylates, polyurethanes (PU), polyvinyl alcohol (PVA), polypeptides, poly- $\beta$ -malic acid (PMLA), poly- $\beta$ -alkanoic acids, trimethylene carbonate, polyanhydrides, polyorthoesters, polyphosphazenes, poly(trimethylene carbonates), PLA-polyethylene oxide (PELA), and tyrosine based polymers.

37. The system of any of Claims 1, 3 or 5 wherein said at least some portion of at least some of said particles of said agent are selected from the group consisting of alginate, calcium, calcium phosphate, ceramics, cyanoacrylate, collagen, dacron, elastin, fibrin, gelatin, glass, gold, hydrogels, Hydroxy apatite, hydroxyethyl methacrylate, hyaluronic acid, liposomes, Nitinol, oxidized regenerated cellulose, phosphate glasses, polyethylene glycol, polyester, polysaccharides, polyvinyl alcohol, platelets, blood cells, radiopaque salts, silicone, silk, steel, synthetic polymers, thrombin, and titanium.

38. A method of vascularizing cardiac tissue of a living being comprising the steps of:

- (a) providing a flowable agent comprising a plurality of small diameter particles; and
- (b) introducing said flowable agent at or adjacent the cardiac tissue by imparting a force to said agent, whereupon said agent directly enters the cardiac tissue at an entry situs.

39. The method of Claim 38 additionally comprising the steps of:

- (c) forming a plurality of channels in the wall of the myocardium at spaced locations from one another and in communication with the interior of the heart; and
- (d) introducing said flowable agent into said channels.

40. The method of Claim 38 wherein at least some portion of at least some of said particles is formed of a material to cause the formation of lumens in communication with the being's arterial system.

41. The method of Claim 39 wherein said channels in the wall of the myocardium are created by the application of energy to the myocardium.

42. The method of Claim 38 additionally comprising the step of applying energy to the myocardium to treat the cardiac tissue.

43. The method of Claim 42 wherein the application of energy to the myocardium produces channels therein.

44. The method of Claim 42 wherein said energy is selected from the group consisting of one or more of mechanical, electrical, thermal, electromagnetic, vibratory, hydraulic, pneumatic, and nuclear energy.

45. The method of Claim 39 additionally comprising applying a biologically active material to the myocardium to result in the production of said channels.

46. The method of Claim 38 additionally comprising the step of monitoring the cardiac cycle of the being and coordinating the introduction of said flowable agent with the cardiac cycle.

47. A method of affecting the conduction of electrical signals in cardiac tissue of a living being comprising the steps of:

- (a) providing a flowable agent comprising a plurality of small diameter particles; and
- (b) introducing said flowable agent at or adjacent the cardiac tissue by imparting a force to said agent, whereupon said agent directly enters the cardiac tissue at an entry situs.

48. The method of Claim 47 additionally comprising the steps of:

- (c) forming a plurality of channels in the wall of the myocardium at spaced locations from one another and in communication with the interior of the heart; and
- (d) introducing said flowable agent into said channels.

49. The method of Claim 47 wherein at least some portion of at least some of said particles is formed of a material to cause the formation of lumens in communication with the being's arterial system.

50. The method of Claim 48 wherein said channels in the wall of the myocardium are created by the application of energy to the myocardium.

51. The method of Claim 47 additionally comprising the step of applying energy to the myocardium to treat the cardiac tissue.

52. The method of Claim 51 wherein the application of energy to the myocardium produces channels therein.

53. The method of Claim 51 wherein said energy is selected from the group consisting of one or more of mechanical, electrical, thermal, electromagnetic, vibratory, hydraulic, pneumatic, and nuclear energy.

54. The method of Claim 48 additionally comprising applying a biologically active material to the myocardium to result in the production of said channels.

55. The method of Claim 47 additionally comprising the step of monitoring the cardiac cycle of the being and coordinating the introduction of said flowable agent with the cardiac cycle.

56. A method of affecting the conduction of nerve signals in cardiac tissue of a living being comprising the steps of:
- (a) providing a flowable agent comprising a plurality of small diameter particles; and
  - (b) introducing said flowable agent at or adjacent the cardiac tissue by imparting a force to said agent, whereupon said agent directly enters the cardiac tissue at an entry situs.
57. The method of Claim 56 additionally comprising the steps of:
- (c) forming a plurality of channels in the wall of the myocardium at spaced locations from one another and in communication with the interior of the heart; and
  - (d) introducing said flowable agent into said channels.
58. The method of Claim 56 wherein at least some portion of at least some of said particles is formed of a material to cause the formation of lumens in communication with the being's arterial system.
59. The method of Claim 57 wherein said channels in the wall of the myocardium are created by the application of energy to the myocardium.
60. The method of Claim 56 additionally comprising the step of applying energy to the myocardium to treat the cardiac tissue.
61. The method of Claim 60 wherein the application of energy to the myocardium produces channels therein.
62. The method of Claim 60 wherein said energy is selected from the group consisting of one or more of mechanical, electrical, thermal, electromagnetic, vibratory, hydraulic, pneumatic, and nuclear energy.
63. The method of Claim 57 additionally comprising applying a biologically active material to the myocardium to result in the production of said channels.
64. The method of Claim 56 additionally comprising the step of monitoring the cardiac cycle of the being and coordinating the introduction of said flowable agent with the cardiac cycle.
65. The system of any of Claims 1, 3 or 5 wherein said particles are constructed so that once they are located within the tissue they tend to resist migration therefrom.
66. The system of Claim 65 wherein said particles are shaped to resist such migration.

67. A system for treated targeted internal tissue of a living being to produce a beneficial effect for the being, said system comprising a delivery instrument and a flowable agent, said flowable agent comprising a plurality of small particles for introduction into the targeted tissue, said delivery instrument being arranged to introduce said flowable agent at or adjacent the targeted tissue by imparting a force to said agent, whereupon said agent directly enters the targeted tissue at an entry situs.

68. The system of Claim 67 wherein at least some portion of some of said particles being formed of a material to cause the beneficial effect.

69. The system of Claim 68 wherein said at least some portion of at least some of said particles of said agent comprises one or more of the group consisting of pharmaceuticals, biologically active materials, growth factors, radioactive materials, and radiopaque materials.

70. The system of any of Claim 67 wherein said system includes means to limit the depth of penetration of said particles into the tissue.

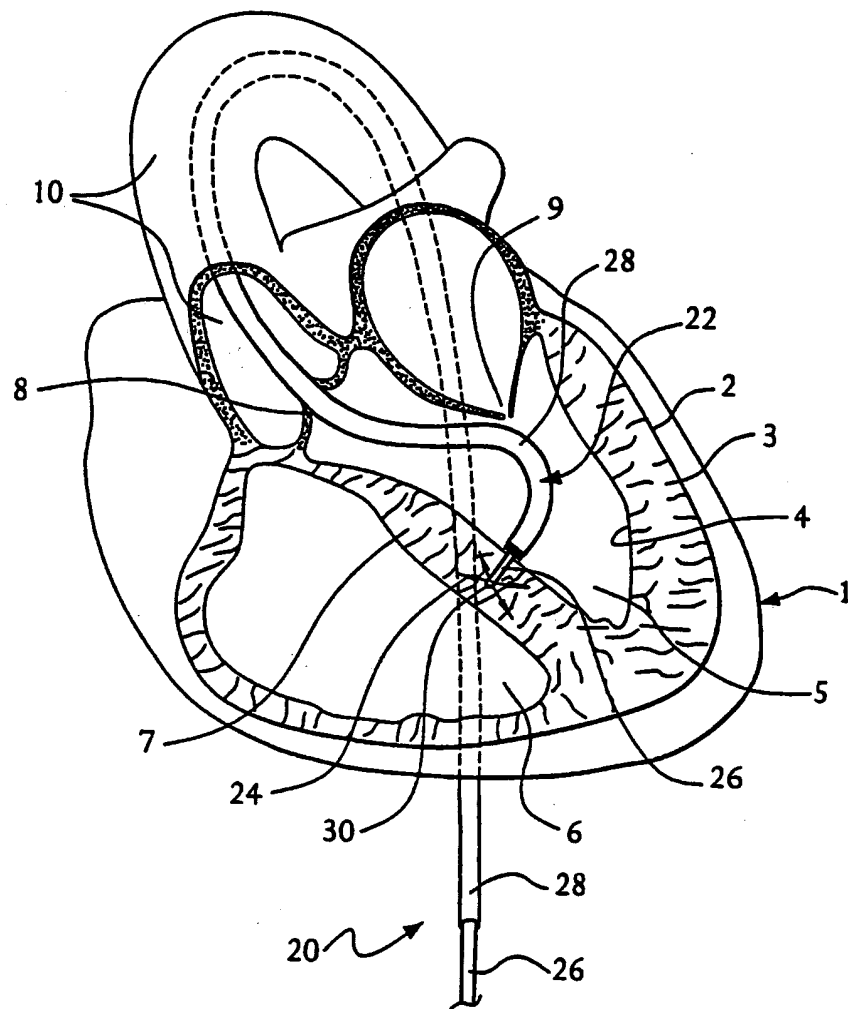


FIG. 1A

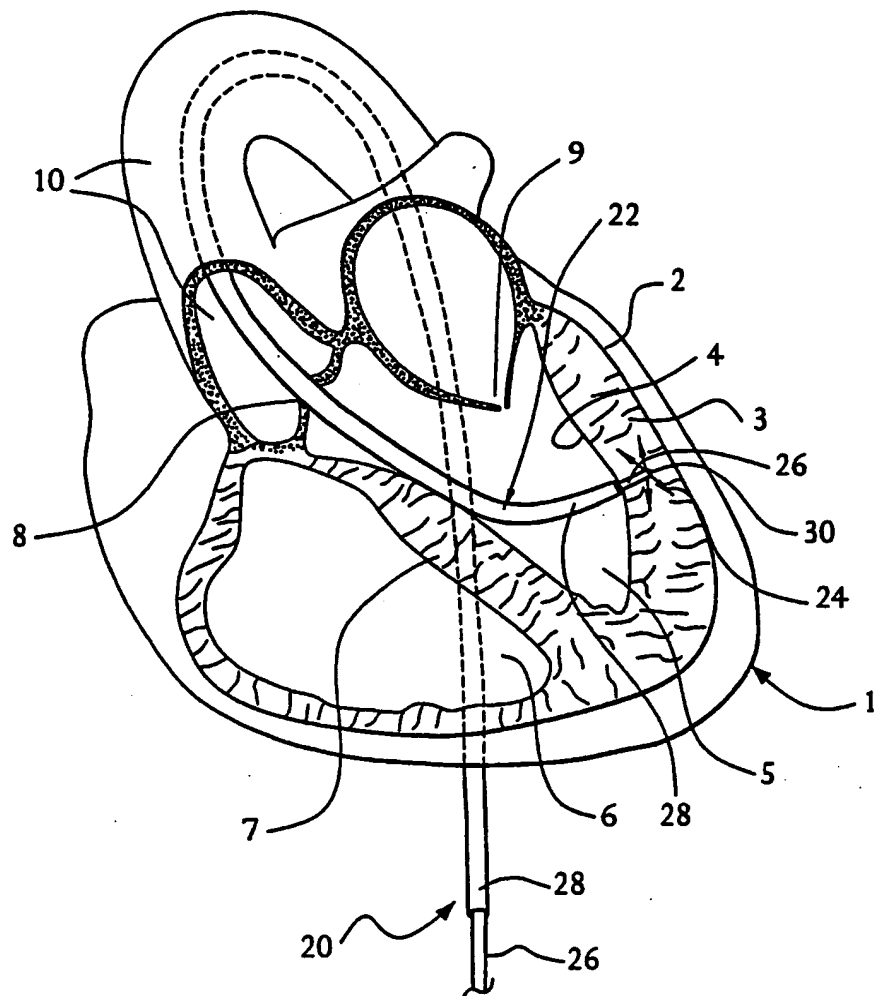


FIG. 1B

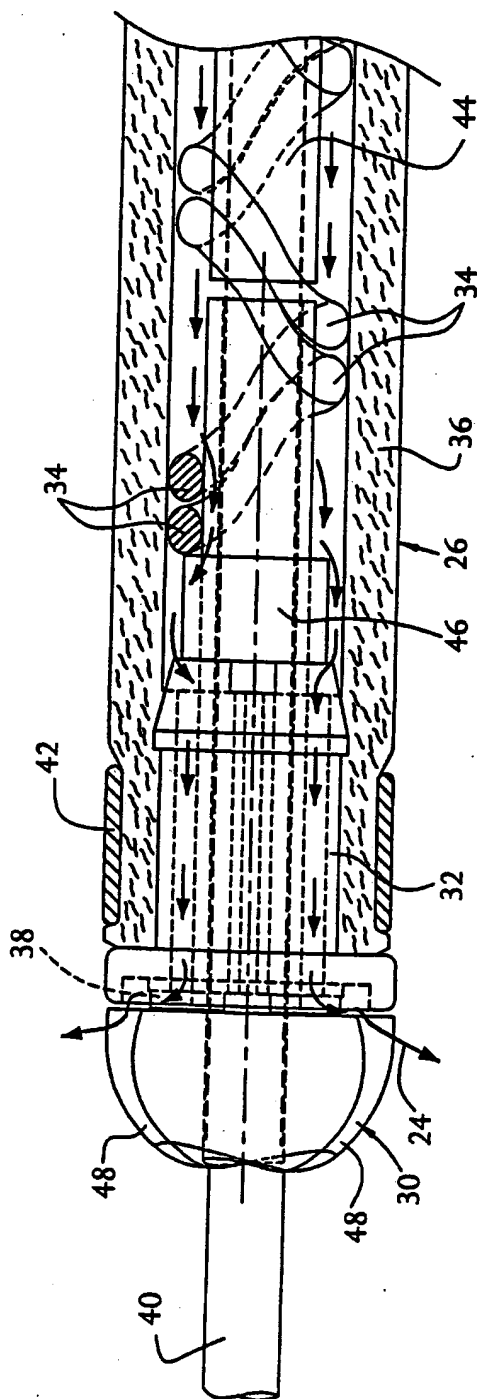


FIG. 2



4/20

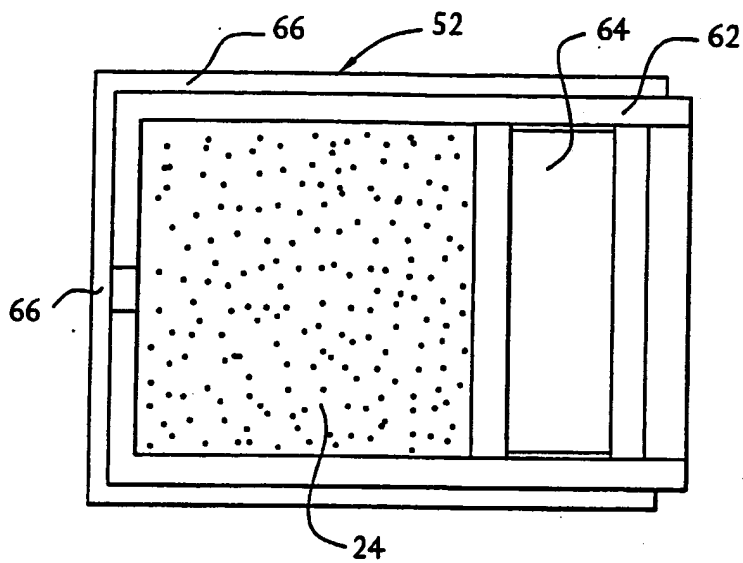


FIG. 3A

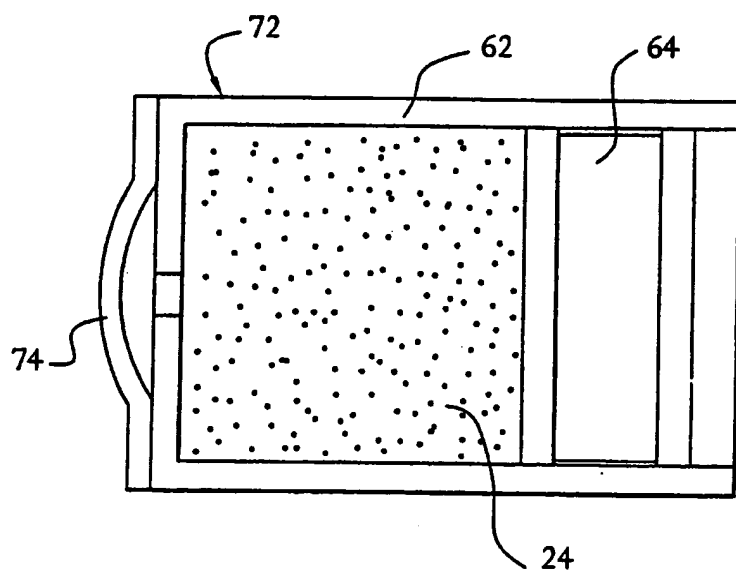


FIG. 3B

5/20

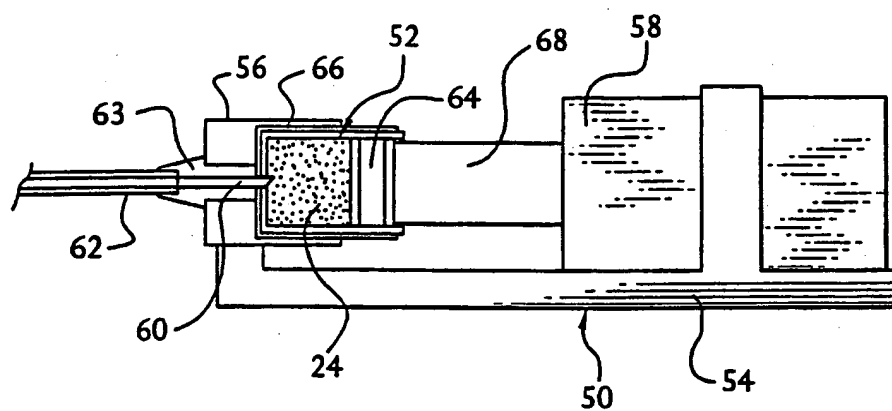


FIG. 4A

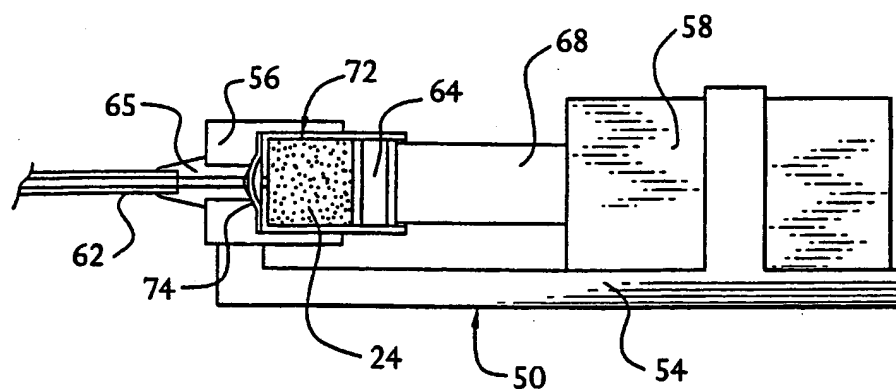


FIG. 4B

6/20

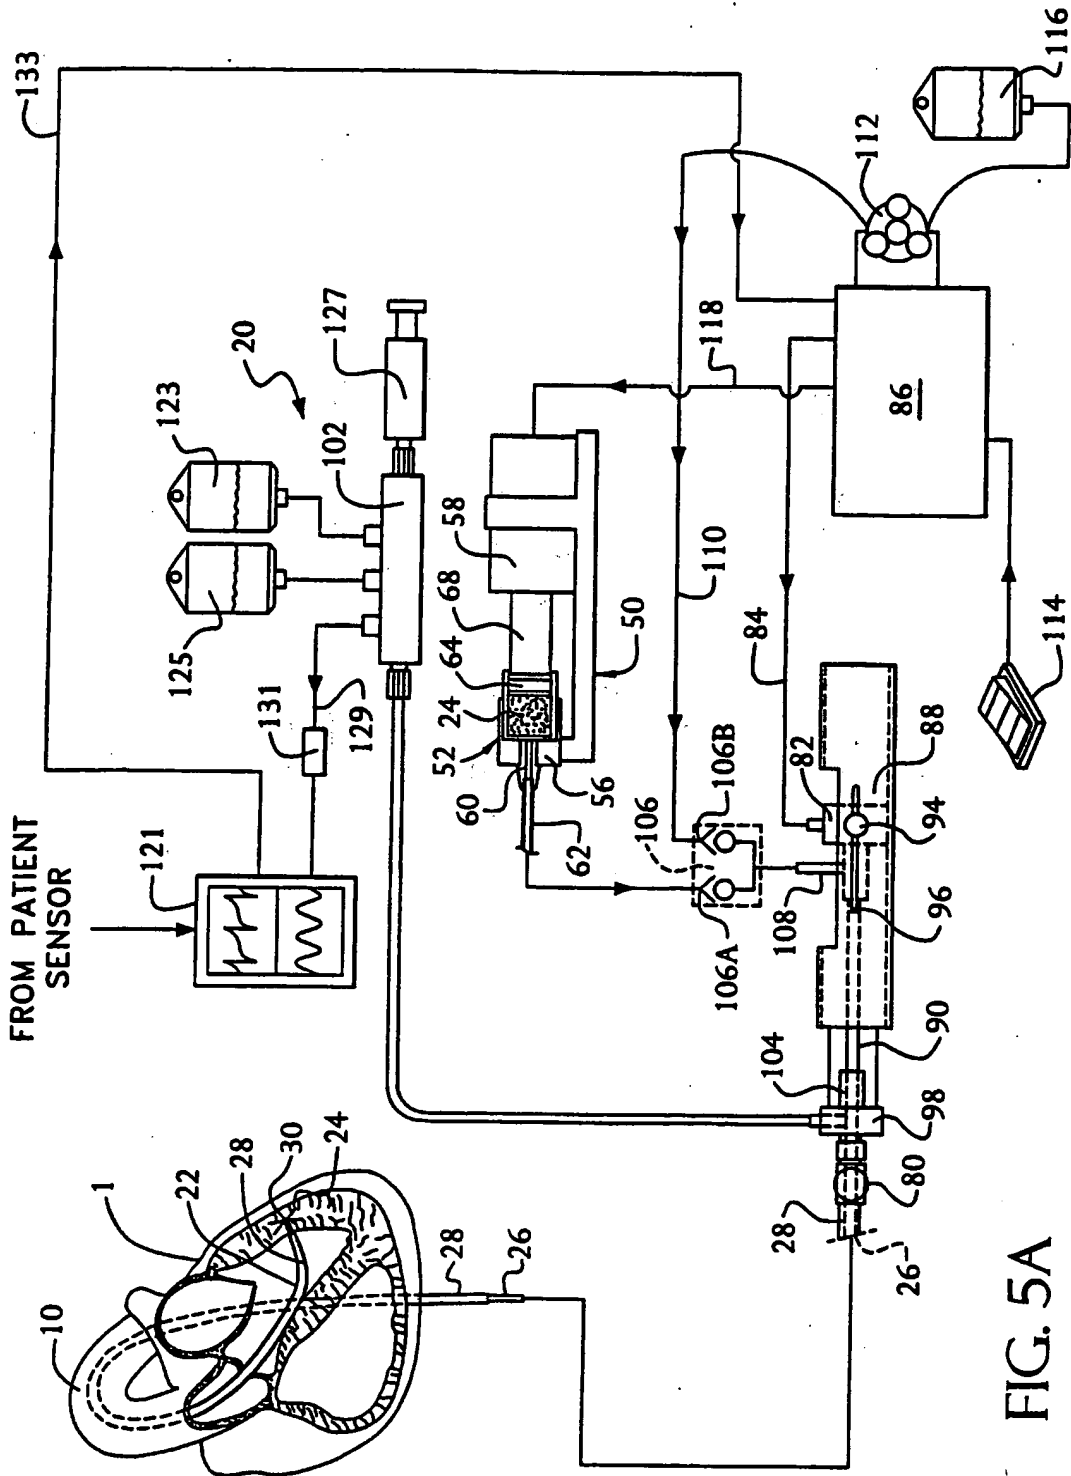


FIG. 5A

7/20

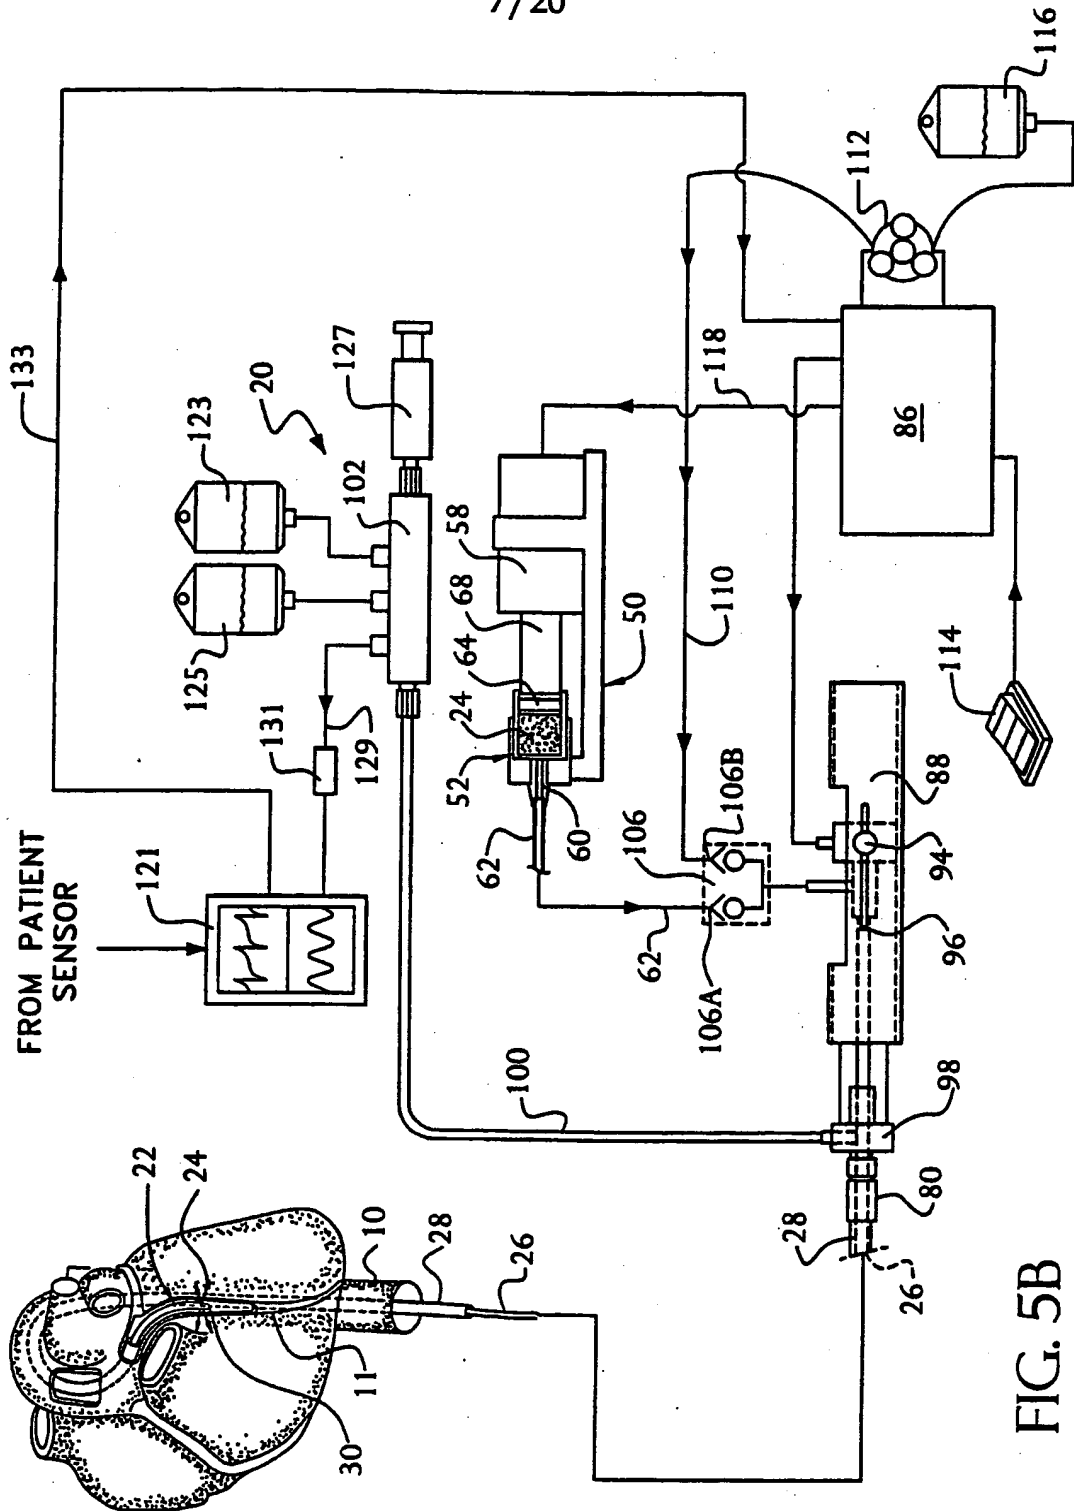


FIG. 5B



9/20

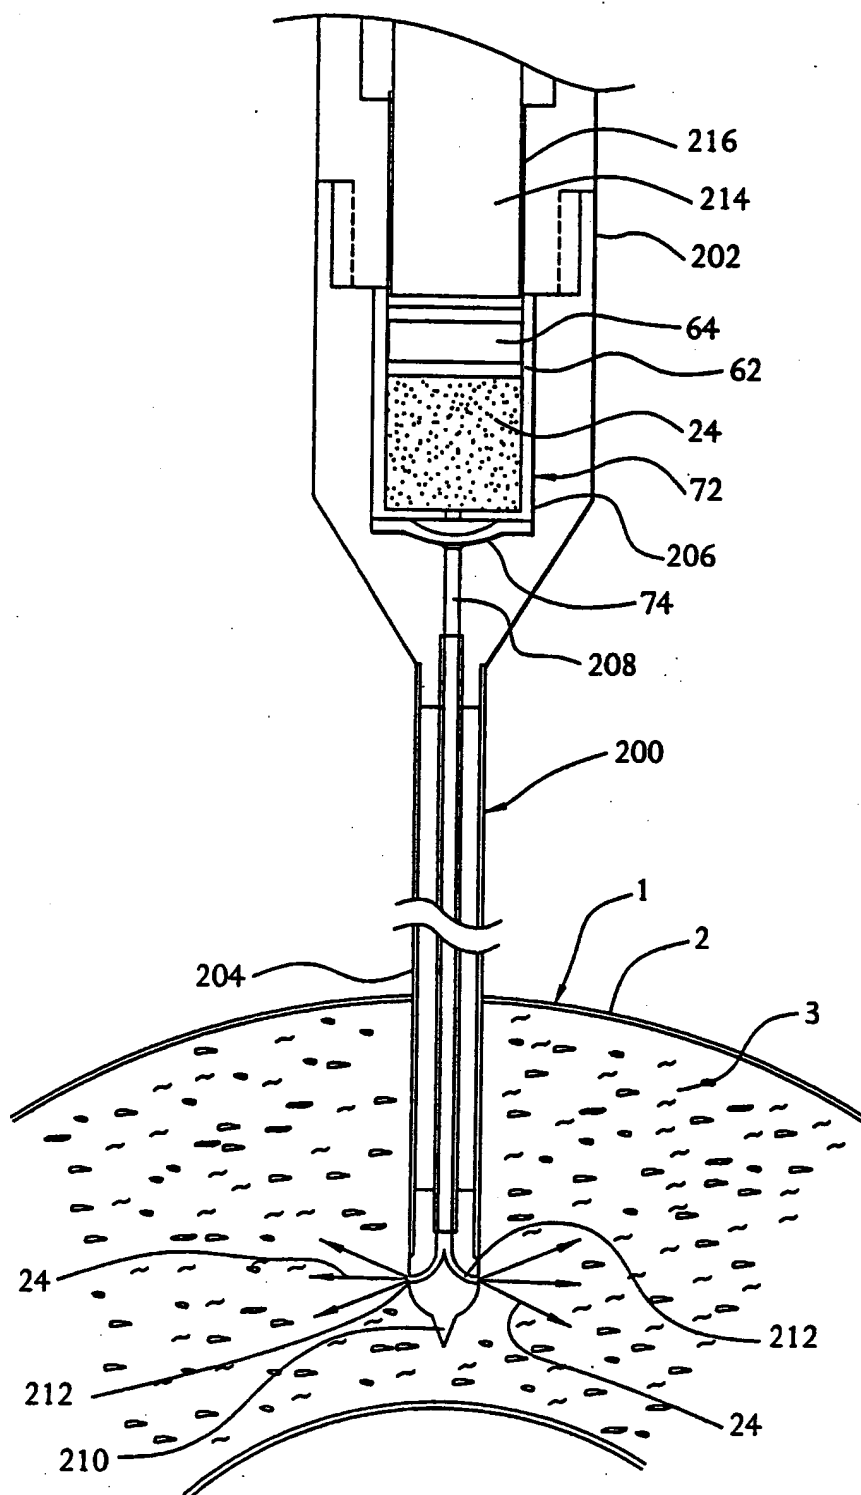


FIG. 7

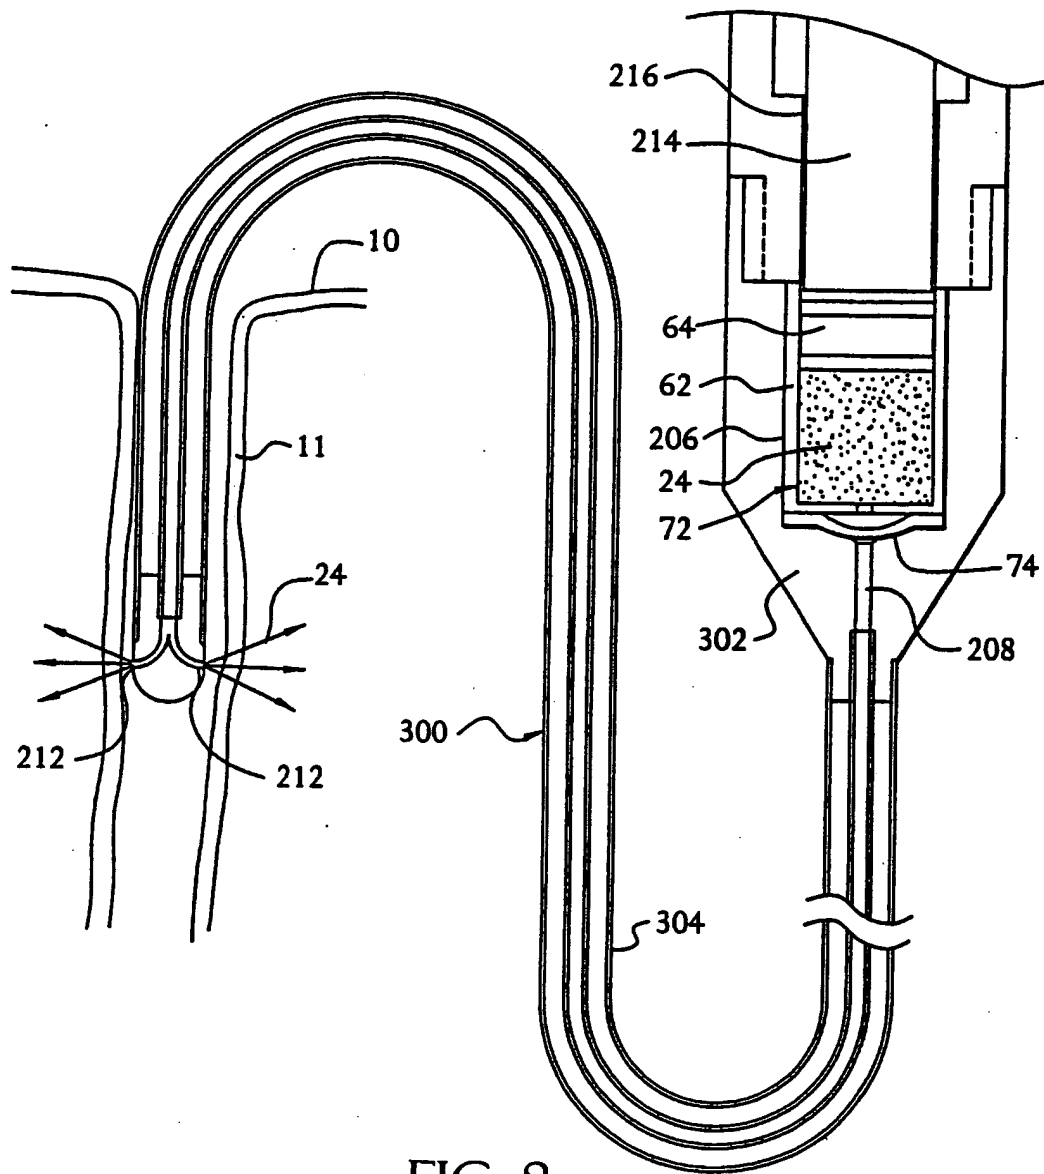


FIG. 8

11/20

FIG. 10

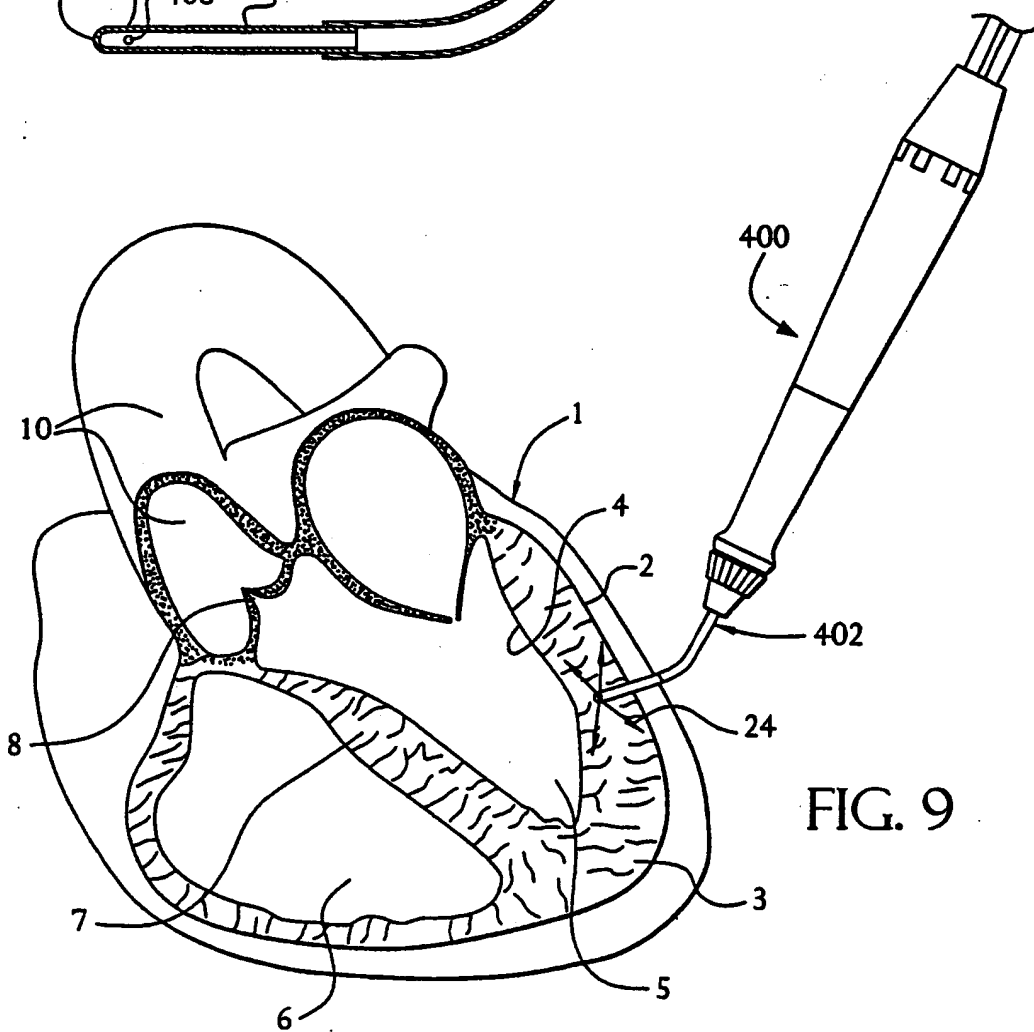
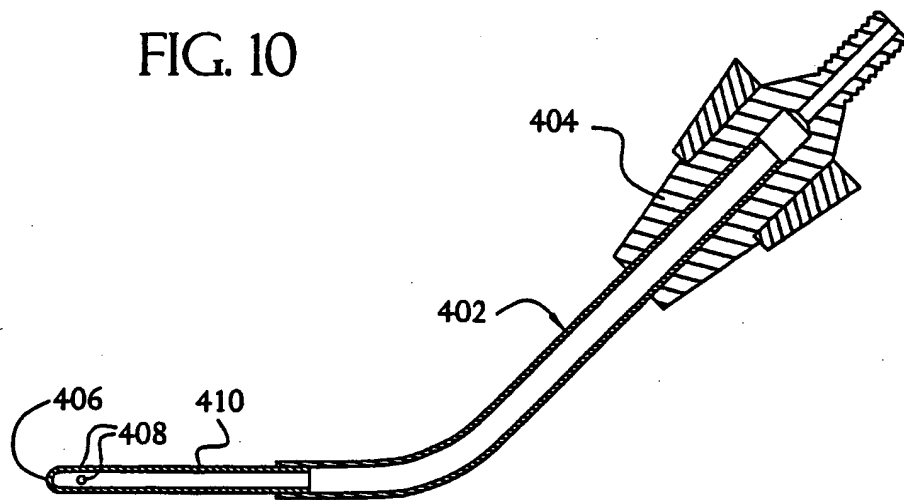


FIG. 9



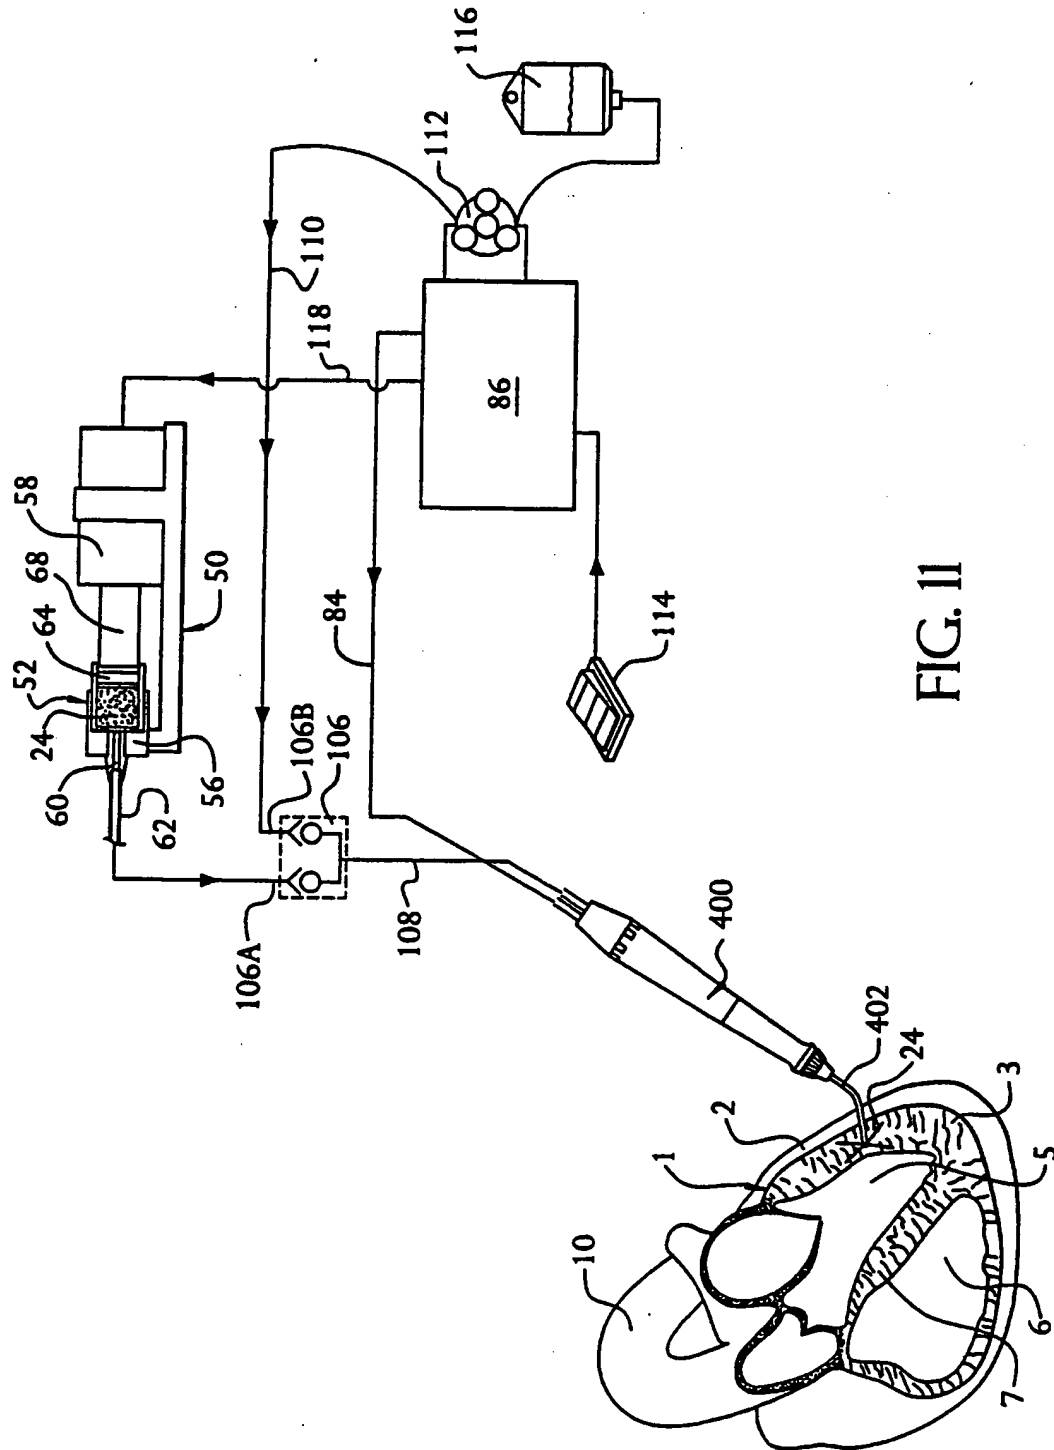


FIG. 11

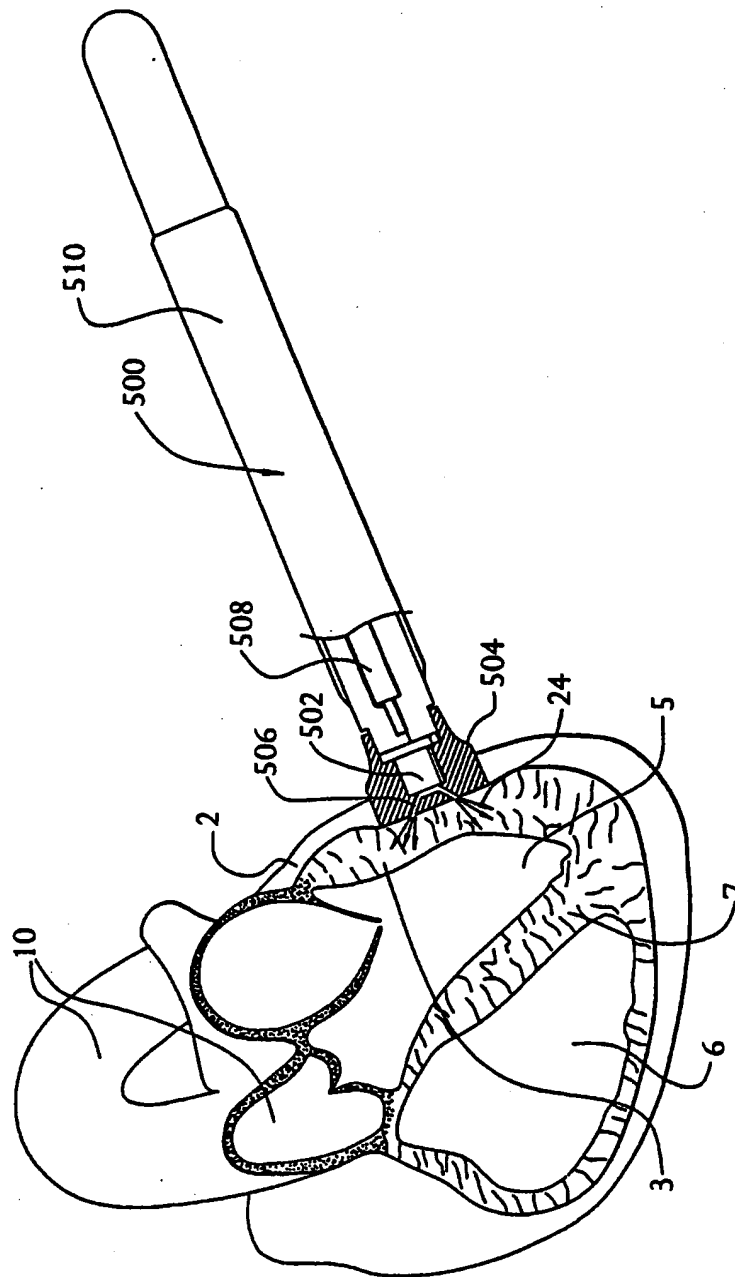


FIG. 12

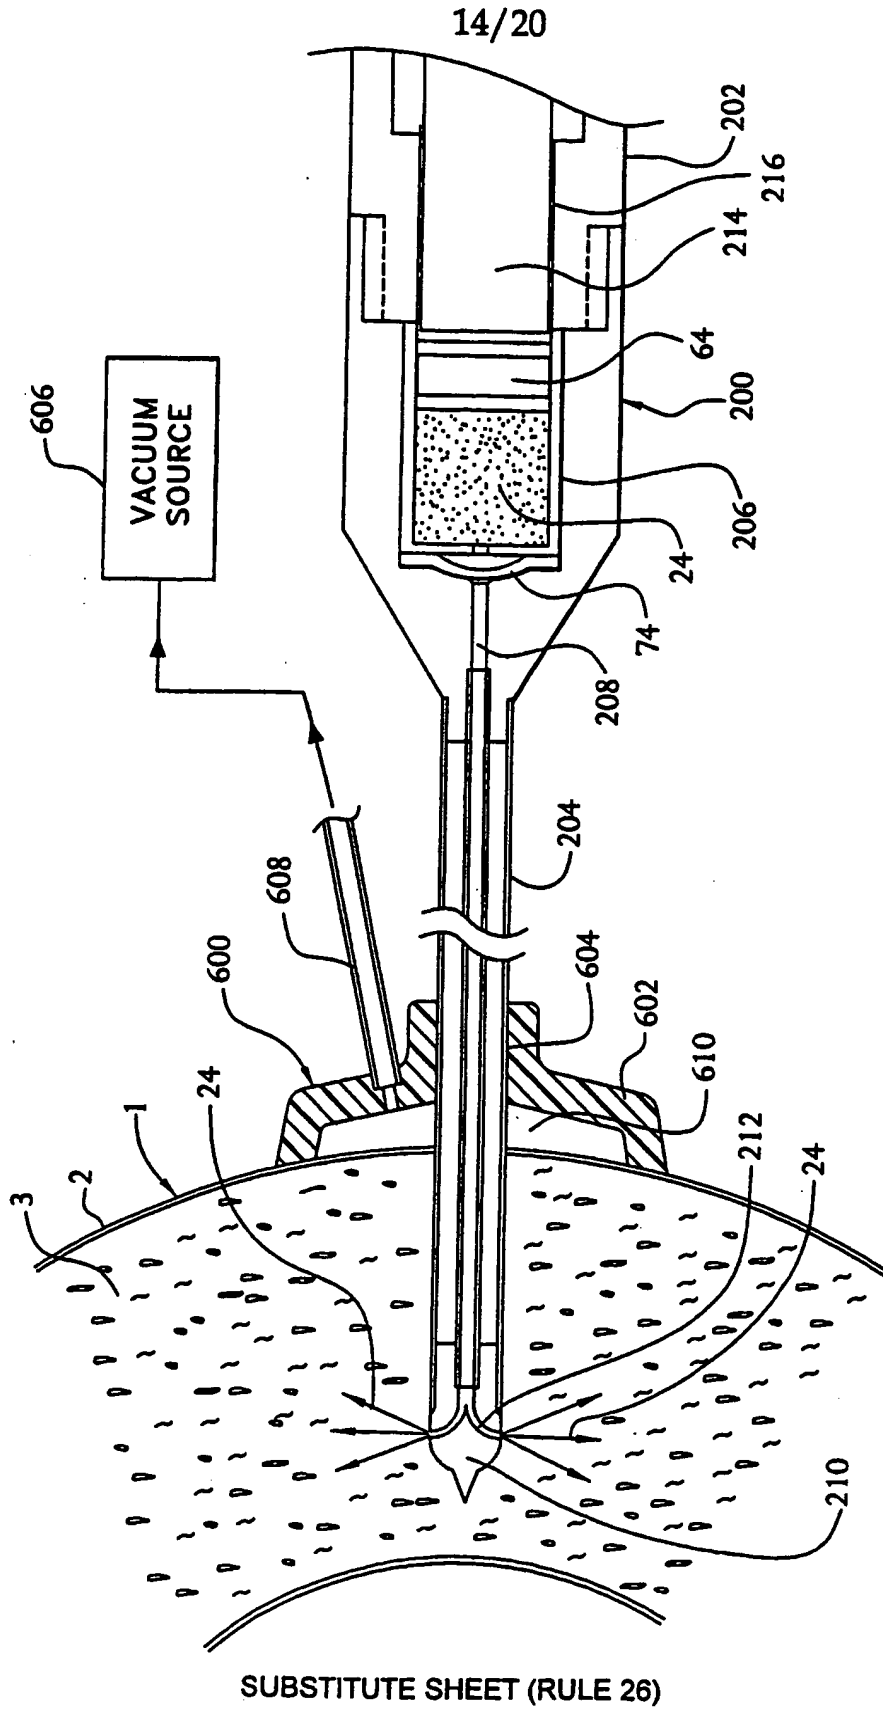


FIG. 13

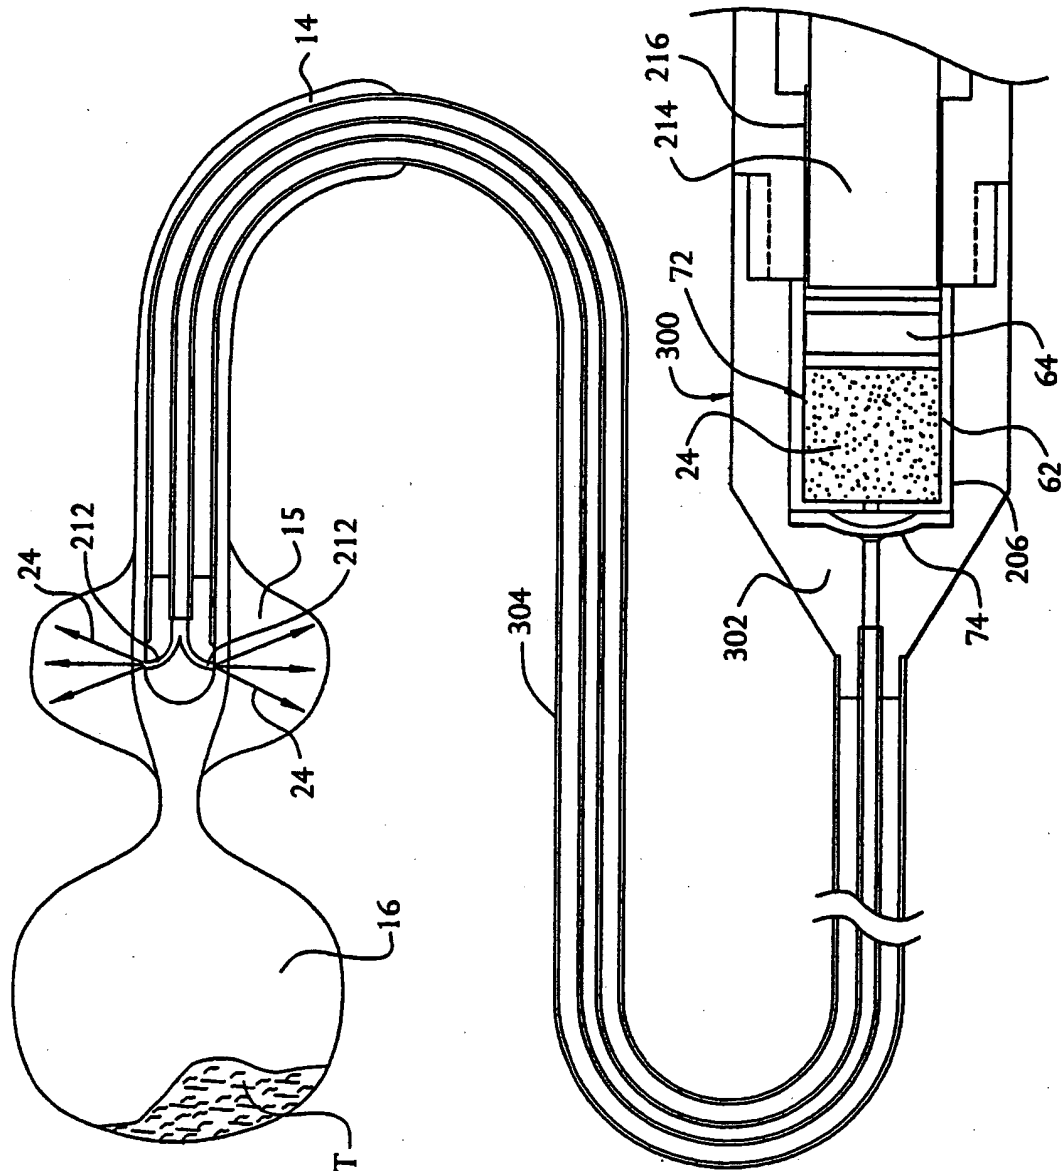


FIG. 14

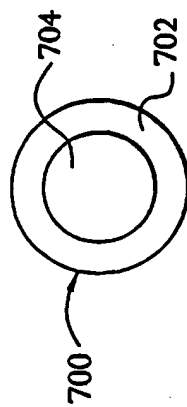


FIG. 15A




FIG. 15B




FIG. 15C




FIG. 15D




FIG. 15E




FIG. 15F




FIG. 15G




FIG. 15H



FIG. 15I

17/20

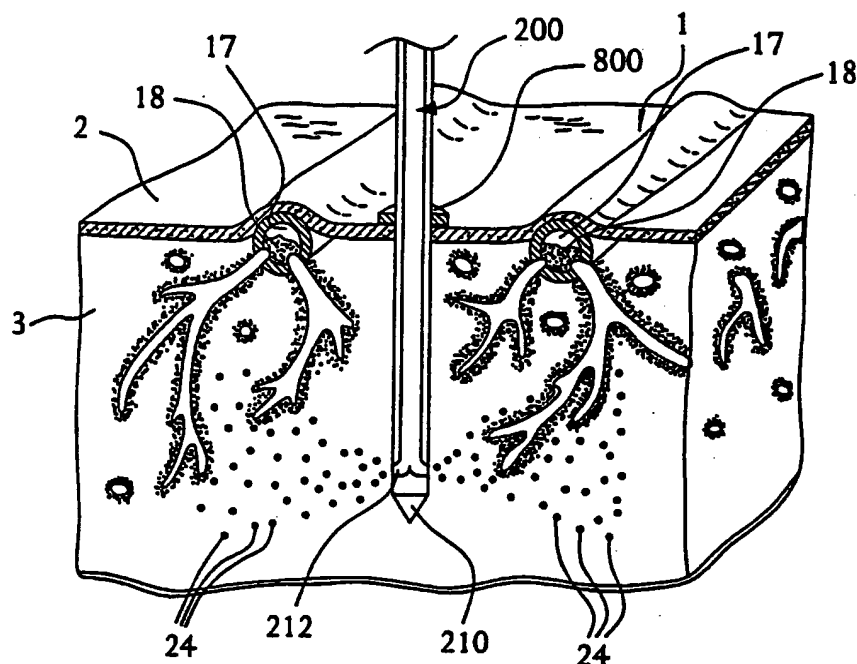


FIG. 16

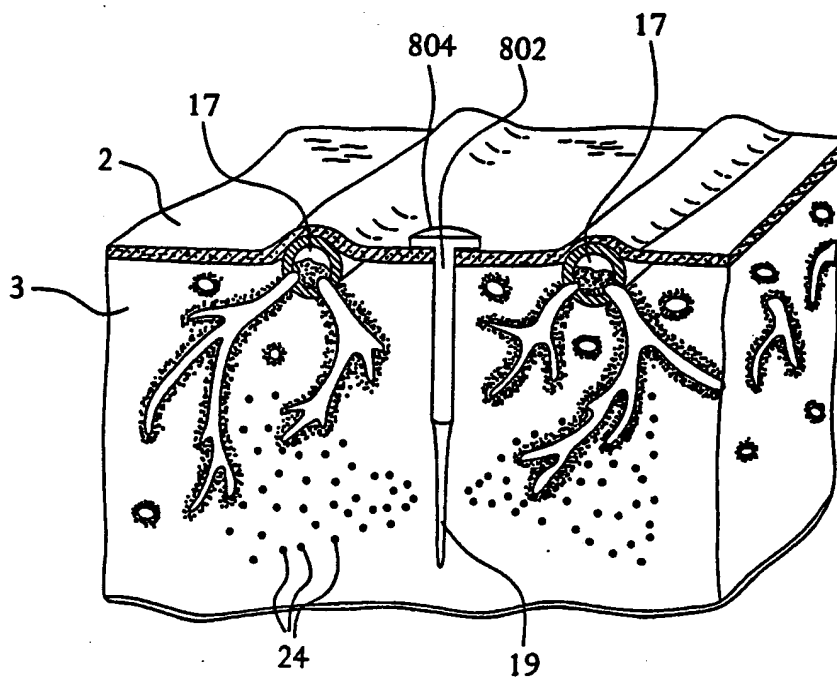


FIG. 17

SUBSTITUTE SHEET (RULE 26)

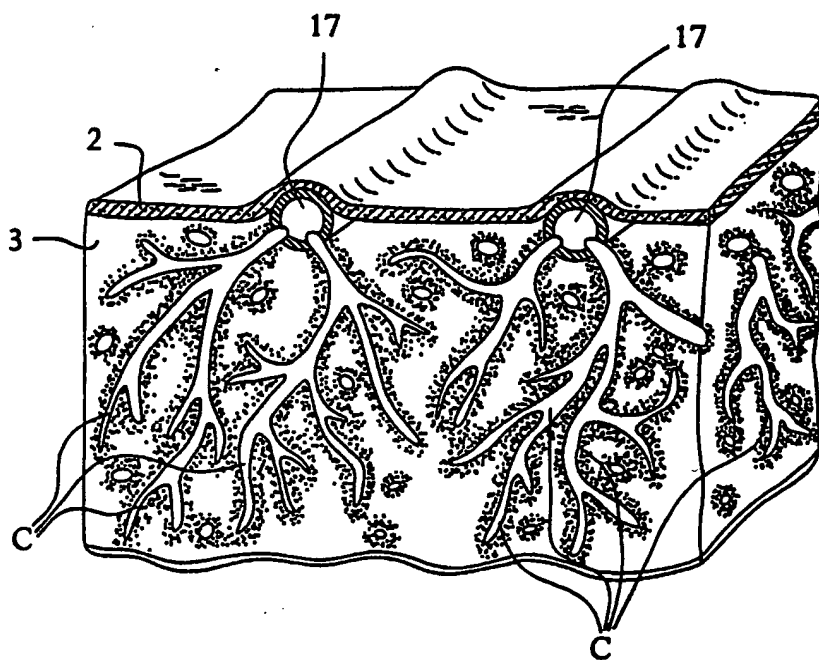


FIG. 18

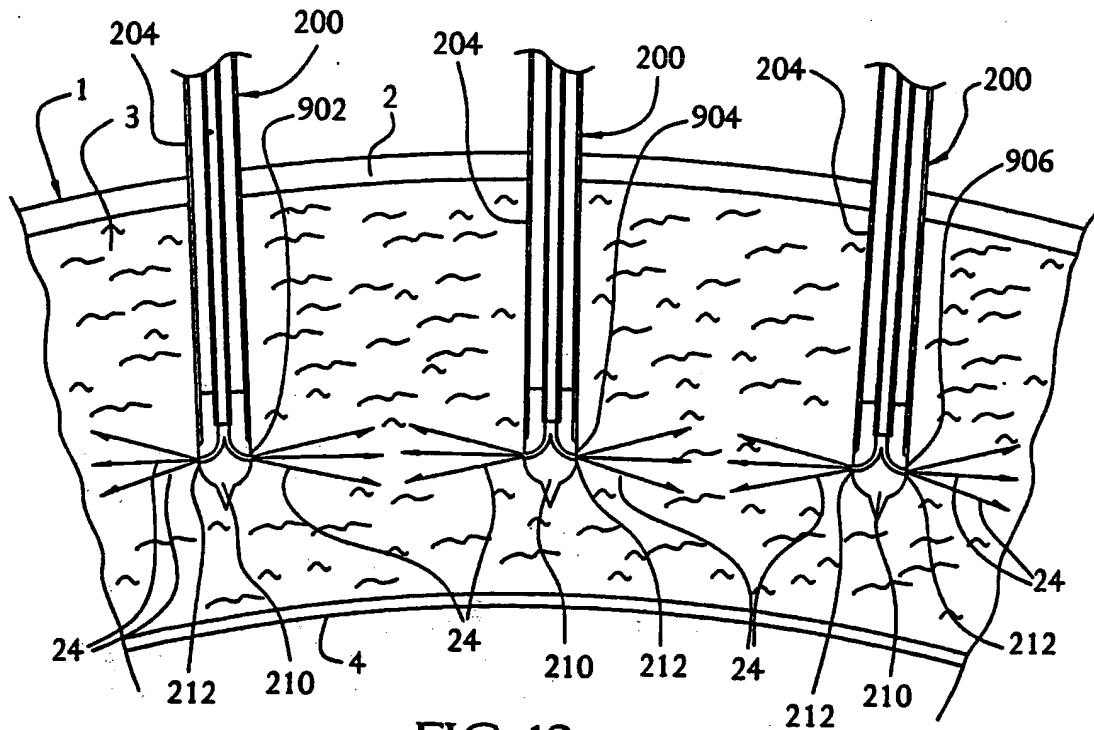


FIG. 19

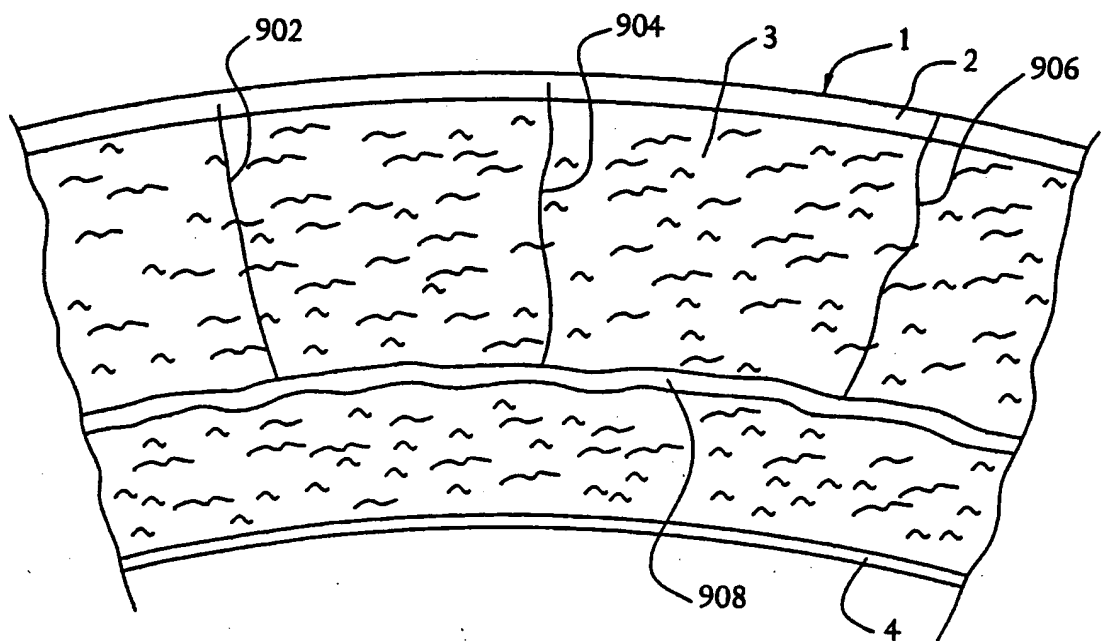


FIG. 20



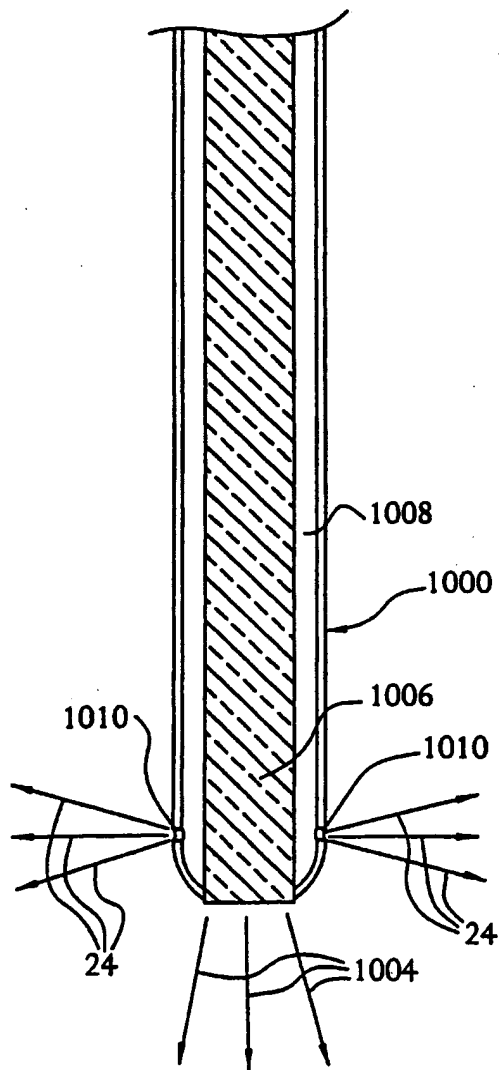


FIG. 21

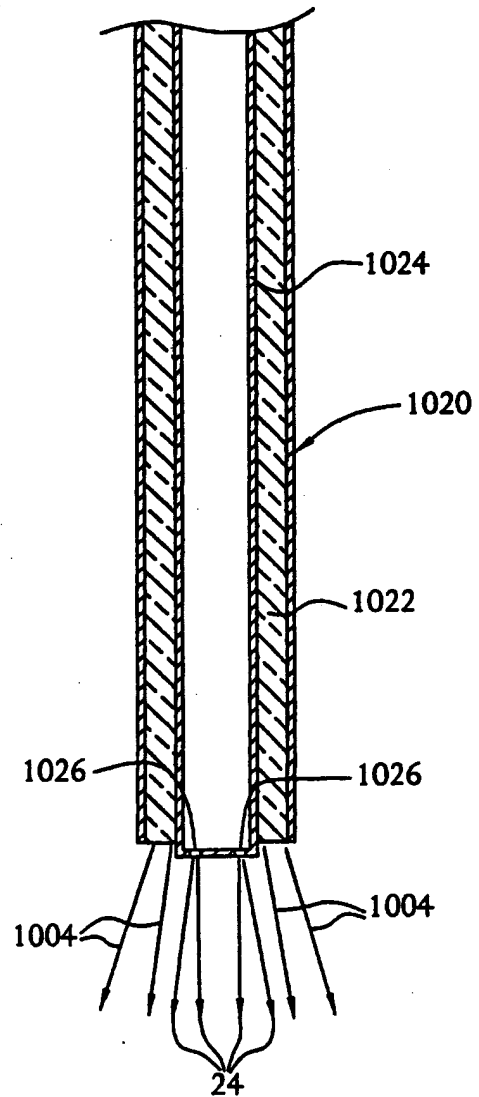


FIG. 22

# INTERNATIONAL SEARCH REPORT

International Application No.  
PCT/US 00/20525

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61B17/22

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, PAJ

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 99 33510 A (FREEMAN DONALD C JR ;STAID KEVIN (US); HYDROCISION INC (US); MOUTA) 8 July 1999 (1999-07-08)  page 5, line 8 -page 7, line 2; figures	1-8,10, 12-17, 19-28, 31,34, 67-69
A	WO 99 22655 A (SCIMED LIFE SYSTEMS INC) 14 May 1999 (1999-05-14) the whole document	1-37, 67-69
A	WO 98 19614 A (FOGARTY THOMAS J) 14 May 1998 (1998-05-14) abstract; figures	1,3,5,67
A	US 5 871 469 A (EGGERS PHILIP E ET AL) 16 February 1999 (1999-02-16) abstract; figures	1,3,5,67

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

### \* Special categories of cited documents:

\*A\* document defining the general state of the art which is not considered to be of particular relevance

\*E\* earlier document but published on or after the international filing date

\*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

\*O\* document referring to an oral disclosure, use, exhibition or other means

\*P\* document published prior to the international filing date but later than the priority date claimed

\*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

\*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

\*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

\*Z\* document member of the same patent family

Date of the actual completion of the international search

12 December 2000

Date of mailing of the international search report

18/12/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax (+31-70) 340-3018

Authorized officer

Kousouretas, I

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No  
PCT/US 00/20525

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9933510 A	08-07-1999	AU 2022199 A EP 1049511 A	19-07-1999 08-11-2000
WO 9922655 A	14-05-1999	US 6045565 A EP 1028661 A	04-04-2000 23-08-2000
WO 9819614 A	14-05-1998	US 6042581 A US 6053911 A AU 7000298 A EP 0984727 A	28-03-2000 25-04-2000 29-05-1998 15-03-2000
US 5871469 A	16-02-1999	US 5697882 A US 5697281 A US 5366443 A US 6066134 A US 6149620 A AU 702687 B AU 1054597 A CA 2237947 A EP 0886493 A JP 2000060868 A JP 11501555 T WO 9718765 A US 5843019 A US 6105581 A US 6113597 A AU 706294 B AU 6026696 A CA 2221330 A EP 0837647 A JP 2912023 B JP 10510745 T US 6032674 A US 6063079 A US 6142992 A US 6053172 A WO 9639914 A US 6086585 A US 5683366 A US 6024733 A US 5810764 A US 5902272 A US 5697536 A US 5860951 A US 5873855 A US 6109268 A AU 711197 B AU 2472497 A AU 676329 B AU 6829694 A CA 2162395 A EP 0697841 A JP 2931102 B JP 9501328 T NZ 266678 A WO 9426228 A US 5681282 A US 5888198 A	16-12-1997 16-12-1997 22-11-1994 23-05-2000 21-11-2000 04-03-1999 11-06-1997 29-05-1997 30-12-1998 29-02-2000 09-02-1999 29-05-1997 01-12-1998 22-08-2000 05-09-2000 10-06-1999 30-12-1996 19-12-1996 29-04-1998 28-06-1999 20-10-1998 07-03-2000 16-05-2000 07-11-2000 25-04-2000 19-12-1996 11-07-2000 04-11-1997 15-02-2000 22-09-1998 11-05-1999 16-12-1997 19-01-1999 23-02-1999 29-08-2000 07-10-1999 14-08-1997 06-03-1997 12-12-1994 24-11-1994 28-02-1996 09-08-1999 10-02-1997 19-12-1997 24-11-1994 28-10-1997 30-03-1999

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US 00/20525

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5871469 A		US 5891095 A	06-04-1999
		AT 173903 T	15-12-1998
		AU 3335793 A	03-08-1993